

Otoport OAE+ABR

User Manual for Otoport Flexi

The Otoport Flexi is a variant of the Otoport DP+TE



Otoport OAE+ABR

Otoport Flexi

Issue 3.5


User Manual for Otoport OAE+ABR

Otoport Flexi

The Otoport Flexi is a variant of the
Otoport DP+TE

Firmware revision: 3.29.1.1 onward

Doc Ref: MANABR3ROW - Issue 3.5

 15/08/2022



Copyright Notice

No part of this publication may be copied by any means,
translated or distributed to third parties without the express
written permission of Otodynamics Ltd.

Copyright © 2022 Otodynamics Ltd. All Rights Reserved.



Otodynamics Ltd
30-38 Beaconsfield Rd
Hatfield Herts AL10 8BB UK



MDSS GmbH Schiffgraben 41,
30175 Hannover, DE



(01) 0 5060396 17249 6
(10) 3.5



Contents

1	Introduction	9
1.1	Intended use	9
1.2	What do OAEs test for	9
1.3	General guidance	10
1.4	General use precautions	11
1.5	Contraindications	12
1.6	Safety	13
1.7	The importance of setting the appropriate stimulus levels	14
1.8	Types of otoacoustic emissions	15
1.9	OAEs and screening	17
1.10	OAEs in the clinic	17
1.11	Auditory Brainstem Response	18
2	Equipment identification	19
2.1	Supplied only in Otoport OAE+ABR kit	19
2.2	Supplied only in Otoport OAE kit	20
2.3	Supplied in both kits	21
2.4	Optional accessories	24
2.5	Controls, indicators and connections	26
2.6	OAE labelling	27
2.7	Otoport OAE+ABR controls, indicators and connections	30
2.8	ABR labelling	31
3	Getting started	34
3.1	Assembling the ABR Module with an Otoport	34
3.2	Removing the Otoport from the ABR Module	37
3.3	Otoport OAE+ABR with non-removable module	37
3.4	Connecting probes and electrodes	38
3.5	Initial charge	40
3.6	Quickstart guides	40
3.7	Using the keys and keypad	44
3.8	Connecting the probe to the Otoport	48
3.9	Disconnecting the probe	49

4	Switching On	51
4.1	Switch on screen	51
4.2	Logo screen	52
4.3	Mode select	53
4.4	Login	54
4.5	Test choice	55
5	Test preparation	57
5.1	General checks before testing	57
5.2	Environment checks for ABR	57
5.3	Tip selection and probe fitting	58
5.4	Electrode fitting	60
6	Test troubleshooting	63
6.1	OAE test problems	63
6.2	ABR test problems	64
7	Test selection	66
7.1	Choose test type or workload	66
7.2	Patient details	68
7.3	Select test ear	69
7.4	Checkfit	70
8	DPOAE test	73
8.1	DP stimulus calibration	73
8.2	DP test screen	74
8.3	Test stop reasons	80
8.4	DPOAE test results	81
9	TEOAE test	82
9.1	TE stimulus adjustment	82
9.2	TEOAE test screen	83
9.3	Test stop reasons	89
9.4	TEOAE test results	91

10	ABR test	92
10.1	Impedance check	93
10.2	Checkfit	97
10.3	Ear cup Checkfit	97
10.4	ABR test	98
10.5	Bilateral ABR testing	105
11	Saving the test	107
11.1	Quick Save option	107
11.2	Patient details	109
11.3	Review	110
11.4	Last	111
11.5	Result	113
12	Link-Test	114
13	Work List	115
13.1	Adding Patients	115
13.2	Editing details	116
13.3	Deleting Patients	117
13.4	Testing from the Work List	117
14	Utilities	118
14.1	Patients tested	119
14.2	Patient details	120
14.3	Summary results	121
14.4	Detailed results	123
15	Configuration	124
15.1	Quality tests	124
15.2	Test settings	125
15.3	Date and time	145
15.4	System	146
15.5	Users	153

16	Printing and downloading	156
16.1	Bluetooth wireless technology enabled printing and download	156
16.2	Wired downloading	157
16.3	When you can print	158
16.4	The printing process	162
16.5	Printer fault detection	164
16.6	Printer light summary	165
16.7	Paper	166
16.8	Charging the printer	167
16.9	Changing the battery	168
17	Quality tests	169
17.1	Probe test	169
17.2	ABR cable test	175
17.3	Cavity test	176
17.4	Occlusion test	177
17.5	Real ear test	178
18	Probe, tips and accessories	179
18.1	Probe and service accessories	179
18.2	Probe cable clip	179
18.3	DPOAE+TEOAE probe tips	181
19	Probe care	183
19.1	Cleaning	183
19.2	Changing probe coupler tubes	183
19.3	Probes safety note	185
20	Care of the Otoport	186
20.1	Use of the Otoport and cleaning	186
21	Power	188
21.1	Battery life	188
21.2	Initial charge	188
21.3	Standby	189
21.4	Battery charge	190
21.5	Charging the Otoport	192
21.6	Conditioning the Otoport battery	195
21.7	Otoport OAE+ABR	196

22	Equipment troubleshooting	197
22.1	Otoport lock-up	197
22.2	Switch on	197
22.3	System details	197
22.4	Instrument fault message	198
22.5	Hardware fault messages	199
23	Training	200
24	Obtaining service	201
25	Calibration	202
26	Mode of operation	203
26.1	DPOAE test	203
26.2	TEOAE test	204
26.3	ABR test	206
27	Technical specifications	213
27.1	Otoport	213
27.2	Electromagnetic compatibility - User Guidance	218
27.3	Electromagnetic compatibility - Technical Description	220
27.4	EN60645-3 conformance notes	223
27.5	ABR Module	225
27.6	End of life management	226
27.7	Symbol explanations	227
28	Index	230

1 Introduction

This manual provides instructions for use for the Otoport Flexi. This includes both the OAE only and the OAE+ABR versions. Both products are variants of the Otoport DP+TE product.

1.1

Intended use

This Otodynamics Otoport/Otocheck OAE+ABR device is indicated for use when there is a requirement to screen for hearing disorders by objective and non-invasive means. ABR, TEOAE and DPOAE screening test results are automatically interpreted and a clear 'Pass' or 'Refer' result is presented to the user. Use of the device is indicated when the patient is unable to give reliable voluntary responses to sound, especially with infants. Use of the device facilitates the early detection of hearing loss and its characterization. Where the individual to be screened is healthy with no medical conditions related to the ear, as in the case of well-baby hearing screening, the user can be a trained screener. In all other cases the user should be an audiologist or medical professional.

The TEOAE and DPOAE analytical functions of the device are indicated when objective non-invasive clinical investigations require the characterization and monitoring of the functional status of the peripheral auditory function. For this purpose the device is intended to be used by audiologists or other audiological skilled professionals. These TEOAE and DPOAE tests are applicable to populations of any age to obtain objective evidence of peripheral auditory function.

1.2

What do OAEs test for

- OAEs test for problems in the peripheral auditory system. It is important to remember that OAEs do not test the whole hearing system, only cochlear function.
- Absence of OAE can be due to cochlear or middle ear dysfunction. Failure to detect any OAEs can also be due to high levels of noise or a blocked or badly fitted probe.

- The presence of OAEs indicates good middle ear function and good transmission of stimulation by outer hair cells inside the cochlea, at the tested frequency.
- Good OAEs do not exclude the possibility of auditory neuropathy or higher neural dysfunctions but these higher level dysfunctions are almost unknown in the well baby population. This is why OAEs have been used as an effective primary screen in hearing screening programmes for decades in many countries.
- Higher level disorders are occasionally present in 'at risk' and NICU babies and for this reason both OAE and ABR screening is recommended for this group.

1.3

General guidance

Each test type provides evidence of normal peripheral hearing function objectively and non-invasively.

The screening functions of this instrument are especially suitable for use with infants. The ABR screening function uses conventional Fsp methodology to detect the response supported by waveform identification (Template Correlation) which is optimised for infants from 34 weeks to 6 months gestational age. Template-free pass criteria for ABR may be selected for use with patients outside this age range (see chapter 15 **Configuration**, section 15.2.9 **Pass criteria**). OAE screening functions include Otodynamics classic Quickscreen TEOAE technology and Rapid DPOAE technology (depending on the model).

The device can be used in a wide range of different environments for example in the well-baby nursery, the NICU, a doctor's office, an audiology clinic, the outpatient clinic or in the home. For optimum results and short test times the room should be quiet and the patient should be very quiet and still during the test. The device will clearly indicate levels of acoustic noise and electrical interference (with ABR). Use this as a guide to improve the testing environment.

The screening functions of the device are intuitive and suitable for operation by trained screeners without specialized knowledge. Testing and interpretation is automated. The TEOAE and DPOAE analysis functions of the device are intended for clinical audiological investigations when objective non-invasive characterisation and monitoring of the functional status of the peripheral auditory function is required. These functions are intended for use as a part of the audiological diagnostic test battery, not as solitary diagnostic tests. The OAE analysis functions provided on

some models are of particular interest to Audiologists, Ear, Nose and Throat specialists, Neurology specialists, researchers and other health professionals concerned with the differential diagnosis of hearing problems, the monitoring of changes to hearing, the conservation of hearing or the detailed measuring peripheral auditory function.

1.4

General use precautions



The Otoport pass criteria are set in the **Configuration** area (see chapter 15 **Configuration**). It is the responsibility of the user to ensure that the pass criteria set meet their requirements.

Measuring OAEs and ABRs requires that the ear is exposed to sound. Whilst the level of this exposure is harmless under normal test conditions, it is not recommended that tests be allowed to continue indefinitely even if there is no result.

The Otoport includes 'stop criteria' which will automatically terminate the test when an OAE or ABR pass has been achieved or within ten minutes.

Whilst this limits the sound exposure in a single test, the user is responsible for limiting the number of separate tests performed on the same ear.

The Otoport has built in signal analysis proven to distinguish true OAEs and ABRs from artefactual signals. Checks should be performed weekly and before each test session to confirm the system continues to operate effectively (see chapter 17 **Quality checks**).

In exceptional circumstances, either an equipment fault or failure to comply fully with the instructions in this manual may result in unreliable test results. Results with total OAE responses greater than 40 dB SPL should be considered highly suspect and should not be relied on.

The probe's coupler tubes which carry sound to and from the ear canal are protected from contamination by the disposable tip. The probe should never be inserted into the ear without a disposable tip attached. Doing so risks damage to the ear by the probe body and contamination of the probe by the ear.

If contamination occurs the coupler tubes must be replaced (see section 19.2 **Changing probe coupler tubes**).

Visually inspect the coupler tubes before use. A blocked sound delivery tube may prevent the Otoport from achieving its target stimulation level and so prevent testing. It may also attenuate certain frequencies and limit the number of pass bands. A blocked microphone tube will prevent the Otoport from sensing the stimulus level in the ear and from detecting the OAE. As a result the Otoport may apply a louder than normal sound to the ear.

Before inserting the probe, the ear should be inspected to ensure that the ear canal is clean and dry and also to establish that there are no contraindications to carrying out the test (see **Contraindications**).

If the ear is not clean and dry the probe may be damaged. This misuse is not covered by warranty.

All surfaces of the Otoport may be cleaned with an alcohol based wipe or cloth with antiseptic fluid. Dry the device immediately with tissue.

Do not allow liquid to enter the instrument.

If additional hygienic protection is required, clear plastic infection control sleeves designed to contain the Otoport during use are available from Otodynamics.

Otodynamics does not guarantee the accuracy of the test results or the tests themselves, if accessories other than those supplied by Otodynamics are used.

1.5

Contraindications

This device should not be used for testing if there is discharge from the test ear, occlusion of the external auditory meatus by wax or other material, or if there is severe otitis externa.

Testing should also not be performed in the case of deformity of, or surgery to the ear or ear canal which might prevent the probe being comfortably fitted or acoustical sealed into the ear canal, unless examined and permitted by an audiologist or doctor.

1.6

Safety



Caution

Connection of a patient to a high frequency (HF) surgical equipment and to the instrument in ABR mode simultaneously may result in burns at the site of the electrodes and possible damage to the instrument.

The Otoport should not be operated in close proximity to shortwave or microwave therapy equipment.

When one or more ABR electrodes are connected to the patient, take care to avoid any contact between the remaining electrodes and any conductive surfaces, such as other equipment. Failure to observe this precaution may result in harmful electrical currents flowing through the patient.

The ABR skin impedance measurement (via stimulation) function is not intended for trans-thoracic use – follow our guidance on electrode placement.

The Otoport should not be used on a patient with an implanted electronic device unless specialist medical opinion has first been obtained.

Anyone who combines charging devices, software, and IT equipment for use with the instrument configures a Medical System, and is therefore responsible for ensuring that the system complies with the safety requirements of the IEC 60601-1 standard.

Otodynamics Ltd. only selects materials for use in its instruments and accessories that have a proven track record of safe use in medical devices.

All materials used in the manufacture of the Otoport and applied parts meet the biocompatibility requirements of ISO 10993; in consideration of the likely nature and duration of contact of each material with both patient and user.

This device should be used only with the leads, electrodes, probes, ear cups and accessories recommended for use by Otodynamics Ltd. which will comply with medical device Biocompatibility/ Safety Standards (EN ISO 10993/ EN 60601-1).

The Otoport instrument is not protected against liquid ingress (rating IPx0) - do not allow liquid to enter the instrument.

Infants and children should not be left unattended with the Otoport or its accessories.

When connecting the Otoport with PCs, printers and servers a secured user network is required.

Observe good Information security management practices per EN ISO/IEC 27001 standard.

If in any doubt, or if further guidance is required, contact Otodynamics or your dealer for support.

1.7

The importance of setting the appropriate stimulus levels

The correct stimulus setting is vital for effective hearing screening with OAEs and ABR. The optimum stimulus level for your screening programme will be one that identifies the vast majority of infants with abnormal ears, but only rarely wrongly reports a healthy normal ear as needing to be referred.

Screening programs differ in their requirement to detect slight losses, and in their capacity to deal with false positives.

Over the decades in which TEOAE have been studied and used for newborn screening, a click stimulus level of '84dBpe' in the ear has been proved effective and efficient, and become the de facto standard for TEOAE screening. The parameter '84dBpe' indicates the peak sound pressure level of the brief click stimulus. It does not represent the hearing level or sensation level.

For DPOAE screening stimulus levels L1/L2 of 65/55dB SPL are most widely used and recommended in the literature as both sensitive to mild losses and as eliciting a robust response from normal ears. This stimulus decibel level does not indicate the hearing level of the stimuli or the sensitivity to hearing loss.

Unlike for TEOAE and DPOAE the stimulus level for ABR screening is expressed relative to the threshold of hearing for healthy ears (indicated by 'dBHL'). The stimulus dBHL must be calibrated on a group of healthy young ears using the specific stimulus format actually delivered by the instrument. It has to be determined experimentally for each instrument and stimulus type. For ABR screening the stimulus level setting is made somewhat higher than the normal threshold level. This is to ensure that normal healthy responses are recordable in a reasonably short time and that the test is only sensitive to clinically significant losses.

Otoport ABR stimulus settings of both 35 and 40dBHL are widely for used newborn screening. The 35dBHL setting gives exceptional sensitivity to slight losses with a somewhat lower specificity than the 40dBHL setting. The 40dBHL setting gives excellent sensitivity to mild losses and higher specificity i.e., there are fewer false positives. Stimulus levels outside of this range are not recommended for regular screening.

Note that the Otoport ABR is not intended for use in diagnostic use. In clinical testing with OAEs a wider range of stimulation levels are used, especially for DPOAEs as part of the diagnostic process.

Never over-stimulate for infant screening.

Over-stimulation will result in mild and some moderate hearing losses being missed.

TEOAEs - never use stimulus levels above 87dBpe for screening,

DPOAEs - never use stimulus level of 70dB SPL or above for screening

AABR - never use stimulus level above 45dBHL for screening.

See the **Test Configuration** section of this manual for more detailed information.

1.8

Types of otoacoustic emissions

Otoacoustic emissions are sounds which can be recorded in the ear canals of functionally normal ears.

This Otoport can make two types of OAE measurements: Transient Evoked OAEs (TEOAEs) and Distortion Product OAEs (DPOAEs).

The difference between the measurements is largely in the means used to generate and measure the emission, rather than in the source of the emission itself.

TEOAEs use a click to briefly stimulate the cochlea across a wide frequency range and record the response from the cochlea.

DPOAEs use a pair of pure tones of specific frequencies (f_1 and f_2) to stimulate the cochlea and record the distortion generated by the tones in the cochlea at a third frequency ($2f_1-f_2$). Different pairs of f_1 and f_2 frequencies are used in turn to acquire emissions from different areas along the length of the cochlea.

The two measurement techniques have different characteristics and so lend themselves to different uses, for example:

TEOAE are rapidly acquired, sensitive to small hearing losses and stimulate the cochlea broadly across the frequency range required for speech and language development. These properties have meant that TEOAE have been widely used in newborn hearing screening programmes.

DPOAE allow testing at higher frequencies and allow emissions to be measured in patients with moderate hearing losses. These properties have lead to their use in recording OAEs in older patients who may have mild hearing losses.

Other applications may benefit from the use of a combination of both tests and a range of stimulus levels.



1.9

OAEs and screening

OAE testing is commonly used as the primary hearing screen in newborns with no known hearing loss risk factors. Failure to show a strong OAE indicates that further testing or observation is necessary.

OAE testing is frequently used as the initial screen within the 'at risk' population. Passing the OAE test indicates that normal middle ear and cochlear function is present. The specific risks must be evaluated to determine whether ABR (auditory brainstem response) testing is necessary, even after a pass at OAE. Certain clinical conditions indicate the possibility of retro-cochlear/neurological disorders which the OAE test cannot detect.

1.10

OAEs in the clinic

Use of Signal to Noise ratio or SNR

- Signal to noise ratio or SNR is a statistical measure of OAE response validity and signal quality, similar to FSP in ABR. It is used as part of the criteria for a screening 'PASS'. Screening requires a high level of confidence that a real response has been seen and an SNR of 6dB or more at several frequencies is normally required for a PASS.
- For clinical and research purposes it is very important to note that SNR is NOT a reliable physiological measurement of OAE strength. It partially depends on OAE strength but it also depends on the amount of noise present and on the duration of the recording.
- Changes in SNR may have NO clinical significance if they are due to changes in noise levels or test duration. Changes in OAE strength (dBSPL) MAY be clinically significant if recorded with the same stimulus levels, a similar probe fitting and with an SNR greater than 6dB.
- Achieving a high SNR is desirable for clinical purposes because it delivers greater accuracy and higher test-retest reliability of the OAE level measurement.
- NOTE: Some instruments allow different NOISE MODES to be selected e.g. Rapid, Moderate or Standard. The NOISE MODE selected will affect the SNR, or rather the time required to reach the desired SNR. See the **Noise Mode** section.
- For accurate measurements of DPOAE levels for clinical purposes we recommend 12dB SNR in Rapid mode, and 6dBSNR in Standard mode.

1.11

Auditory Brainstem Response

Auditory Brainstem Response (ABR) is an electrophysiological response that measures the auditory system's response to sound. Three voltage sensors (electrodes) are placed on the patient and a sound probe is placed in the test ear. The equipment sends a click, brief tone, or chirp sound stimuli to the test ear.

The cochlea (inner ear) converts sound into electrical signal. These signals travel in sequence to the acoustic nerve, the brainstem, and finally to the cortical areas of the brain. The electrodes pick up these electrical responses to the sound which are commonly known as auditory evoked potentials. A response which occurs within 20ms of the onset of the stimulus is referred to as an Auditory Brainstem Responses (ABR).

As the amplitude of the ABR is very small compared to the 'noise' of other brain electrical activity (EEG) the 'signal to noise ratio' is very poor. It is enhanced by a process called averaging. The amplitude of the ABR is also quite small compared to voltages generated by myogenic (muscle) activity; therefore, ideally, patients should be tested when sleeping or when very still.

If EEG and myogenic artefacts are below a tolerable (noise reject) level, the Otoport ABR firmware will detect the ABR and automatically give a simple Pass/Fail response to the user. Other details of the test including the ABR waveforms may also be viewed, and results interpreted, manually if so desired.



2 Equipment identification

2.1 Supplied only in Otoport OAE+ABR kit

REF FLX-S+ABR

Otoport Flexi OAE+ABR



REF ABR-EC1

Snap electrode cables - 1m

REF ABR-EC2

Snap electrode cables - 2m



REF ABR-SK

Starter kit of snap electrodes (pack of 25), skin preparation gel, pack of cotton wool pads and ear cups



REF ABR-CAV

Probe cavity and ABR cable tester



REF ABR-DS

ABR Desktop stand / Crib hook

Desktop stand / crib hook insert for ABR sleeve.



REF OP-CHG

Charger and mains lead

Supplied with required country-specific plug adapter



REF ABR-INF

Infection control sleeve for Otoport OAE+ABR unit only

Shown fitted



REF ABR-CAS

Equipment case for Otoport OAE+ABR kit




2.2

Supplied only in Otoport OAE kit

REF FLX-S

Otoport Flexi

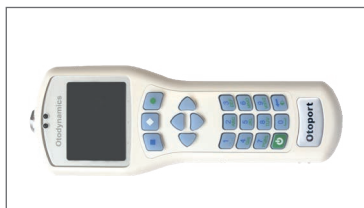

REF OP-CAS

Equipment case for Otoport
Flexi kit



REF ABR-CAV

Probe test cavity



REF OCC

Charging cradle

Not compatible with OAE+ABR
Supplied with required country-specific
plug adapter



REF OP-INF

Infection control sleeve for
Otoport only

Shown fitted



2.3

Supplied in both kits

REF PR-UGD

UGD DPOAE probe



REF PR-POUCH
Drawstring probe pouch



REF PR-CLIP
Probe cable clip



DPC probe coupler tubes x 5

See chapter 19 for fitting instructions

Re-order codes:


REF DPC-10 (quantity: 10)

REF DPC-100 (quantity: 100)



REF BGD
BGD probe body and lid x 1

Re-order quantity: 10

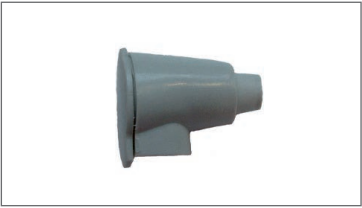

REF DP-BOX
Sample probe tips

See chapter 18
Probe, tips and accessories
for re-order codes



REF OP-CAB
PC download cable



REF OTOLINK
Otolink software CD



Documentation pack

Includes instrument and software manuals, quickstart and probe use guides



Optional accessories

REF ODS

Docking station

- Optional accessory for Otoport Flexi
- Not compatible with or supplied with Otoport Flexi OAE+ABR
- Provides connections for printing, charging and downloading to PC
- Supplied with country-specific plug adapter



REF OMP

Otoport Flexi printer

- Wired and wireless models available for Otoport Flexi
- Wireless model available for Otoport Flexi OAE+ABR



REF OP-CHG

Charger and mains lead

Optional for Otoport OAE kit
Supplied with required country-specific plug adapter



REF OPP-CAS

Large equipment case


For use with Otoport Flexi, with additional compartment for printer



REF ABR-CUP

Ear cups

Optional accessory for ABR screening as an alternative to direct probe use

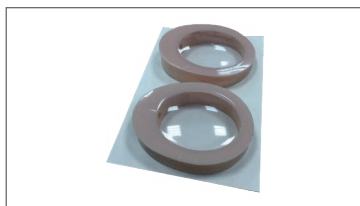

2.4.1

Printer accessories and consumables

REF OMP-CAB

Otoport printer cable

For use with Otoport OAE device
(not for use with ABR)



REF OMP-CHG


Otoport printer charger



REF OMP-PAP

Otoport printer paper rolls

Quantity: 10




REF OMP-SA-PAP

Otoport printer self-adhesive paper rolls

Quantity: 6




2.5 Controls, indicators and connections

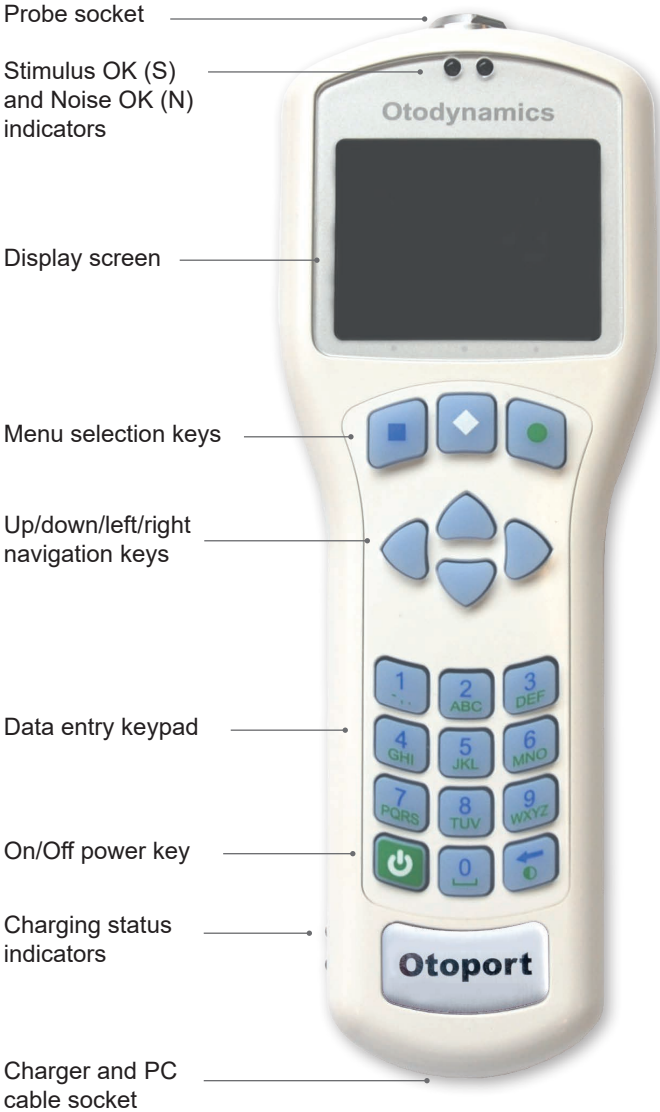

2.6

OAE labelling

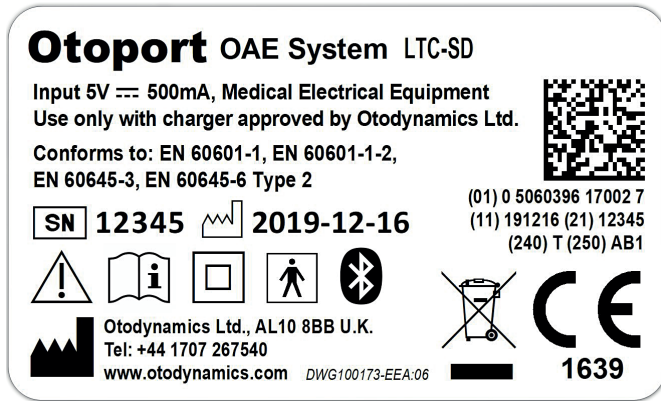



2.6.1

Symbols

The label uses one or more of the following symbols:

Symbol	Description	Where indicated
	DC	Product Label
	Serial Number	Product Label
	Date of Manufacture	Product Label
	Bluetooth® wireless technology enabled	Product Label
	Caution	Product Label
	Refer to user manual	Product Label
	Class II electrical protection (double insulated)	Product Label

continued ...

Symbol	Description	Where indicated
	Type BF applied part	Product Label
	Manufacturer	Product Label

Note:

The Bluetooth® word mark and logos are registered trademarks owned by Bluetooth SIG, Inc. and any use of such marks by Otodynamics Ltd. is under license. Other trademarks and trade names are those of their respective owners

2.6.2

Serial number

The Otoport Flexi OAE system complies with the unique device identifier system to aid the identification of medical devices within the healthcare supply chain.

The fields in the serial number are made up of the following parts:




- (01) Company prefix: Otodynamics, Item reference: Otoport Flexi OAE
- (11) Production date: 31st January 2015
- (21) Serial numbers: 1234 (Otoport)
- (240) Additional product ID: BRT (used to identify any hardware modules fitted)
- (250) Secondary serial number: AB1 (This is a proprietary electronic device identifier, called GSN).

This information is also contained in the adjacent barcode.

2.6.3

Certification or regulatory marks

The label features one or more of the following certification/regulatory marks:

Symbol	Description
	CE Mark (with Notified Body number) (EEA)
	WEEE Directive applies (EEA)
	MET Mark

2.7 Otoport OAE+ABR controls, indicators and connections

Probe sockets and electrode sockets



Impedance check indicator LEDs



Quick-release clips

Otoport unit

Otoport controls and keypad

'USB/PSU' connected' and
'battery charging' indicator LEDs

Charger / PC cable socket




2.8 ABR labelling

2.8.1 System



2.8.2 Upgrade

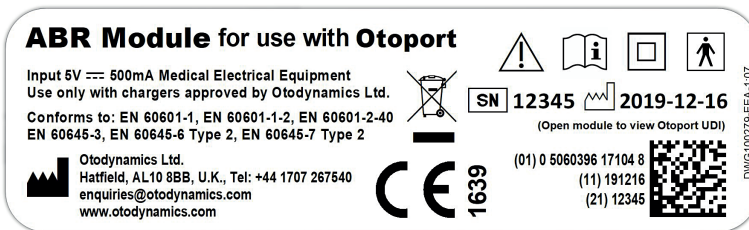






2.8.3 Symbols

The label and device use the following symbols:

Symbol	Description	Where indicated
	DC	Product Label
	Caution	Product Label
	Refer to user manual	Product Label
	Class II electrical protection (double insulated)	Product Label

continued ...

Symbol	Description	Where indicated
	Type BF applied part	Product Label
	Manufacturer	Product Label
	Serial Number	Product Label
	Date of Manufacture	Product Label
	Consult Accompanying Documents (MANDATORY) <i>Safety information should be read and guidance followed, before instrument use.</i>	Device

2.8.4

Serial number

The Otoport Flexi OAE+ ABR system complies with the unique device identifier system to aid the identification of medical devices within the healthcare supply chain.

The fields in the serial number are made up of the following parts:




- (01) Company prefix: Otodynamics, Item reference: Otoport Flexi OAE+ABR
- (11) Production date: 31st January 2015
- (21) Serial numbers: 1234 (Otoport) - 1234 (ABR) (if ABR module is supplied)
- (240) Additional product ID: BRT (used to identify any hardware modules fitted)
- (250) Secondary serial number: AB1 (This is a proprietary electronic device identifier, called GSN).

This information is also contained in the adjacent barcode.

2.8.5

Certification or regulatory marks

The label features one or more of the following certification/regulatory marks:

Symbol	Description
	CE Mark (with Notified Body number) (EEA)
	WEEE Directive applies (EEA)
	MET Mark

3 Getting started

If you have purchased the ABR Module as an upgrade to your Otoport, you will first need to assemble the equipment, as follows.

3.1 Assembling the ABR Module with an Otoport

The ABR Module is designed to be fitted as a 'sleeve' to an Otoport unit, as described in the following instructions:

Do NOT force the Otoport into the ABR sleeve.

- 3.1.1 Lift up the clips on each side of the ABR Module.




- 3.1.2 Hold the lower half of the ABR Module with one hand and use the other hand to slide the upper section up.



- 3.1.3 Slightly tilt the upper section back (see diagram on label inside Module).

Do NOT tilt it forwards and do NOT force it back.

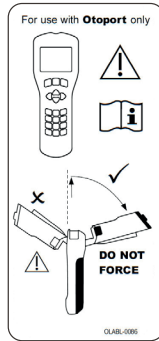

- 3.1.4 Carefully insert the Otoport into the sleeve and slide it down until the connector at the bottom of the sleeve is inserted into the port at the bottom of the Otoport



- 3.1.5 Tilt the upper section of the ABR Module forward (so that it is level with the Otoport)



Please see next page for warning of possible damage if the Otoport is not inserted according to these instructions.

Do NOT insert the Otoport into the top of the module first, or insert into the bottom of the sleeve at an angle, as this may cause damage.



- 3.1.6 Lower the sleeve until the connector at the top of the ABR Module is inserted into the Otoport.



- 3.1.7 Close the clips.



3.2 Removing the Otoport from the ABR Module


If you need to remove the Otoport from the ABR Module at a later time, carefully follow these steps:

- 3.2.1 Open the clips on each side.
- 3.2.2 Slide the top half of the ABR sleeve up and tilt it back.
- 3.2.3 Move the Otoport up to disconnect it from the port at the bottom of the sleeve and remove it from the Module. Do NOT tilt the Otoport forward while lifting it up.

3.3 Otoport OAE+ABR with non-removable module

If you have purchased an Otoport OAE+ABR with a permanently fitted sleeve, sometimes referred to as 'locked', it is not possible to remove the Otoport from the module.

The clips on the side of the locked module are flat.



Non-release clips on 'locked' module

The clips on the unlocked module are shaped for ease of opening.



Quick-release clips on 'unlocked' module

3.4

Connecting probes and electrodes

The connections panel for probes and electrodes is found at the top end of the module.



3.4.1

Connecting the probe

Follow instructions for connecting the probe to the Otoport in section 3.7.

If you are using two probes, ensure that the probe head colour matches the probe socket; the probe with the red head should be connected to the red socket and the blue head to the blue socket.



Some Otoport models only allow a single probe connection to probe socket one. In this case, one probe socket will be blocked.



3.4.2

Connecting the electrodes

The Otoport OAE+ABR is supplied with an electrode cable loom featuring snap stud connectors for electrode attachment. Alternatively, any wired electrodes that are terminated with 1.5mm 'Touchproof' DIN 42-802 connectors may be used.

Carefully align the electrode connector plug with the appropriate electrode socket (observe colour coding) and then push in firmly.



To disconnect the electrode connector, grasp the plug body and pull straight out from the socket.

Important note:

Do not unplug by pulling on the electrode cable as this may damage the cable/plug assembly.

3.5 Initial charge

Before using your Otoport for the first time, fully charge the unit. See chapter 21 **Otoport Power** for details.

3.6 Quickstart guides

Quickstart guides for OAE and ABR tests, included as separate items in your document pack, are shown on the following pages.


OAE QUICKSTART



Otoport Flexi


Step 1. Setting up your Otoport



- 1 With the arrow at the front, connect the DP (grey) probe and screw the knurled sleeve until finger tight.



- 2 Press the  button to turn on the Otoport. Confirm within 2 seconds by pressing the  button.

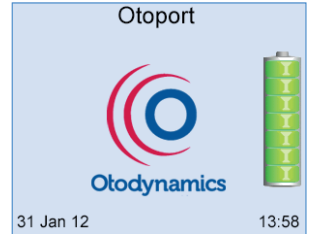

- 3 Date, time and battery status are displayed while system checks are performed.

Step 2. Fitting the earpiece



- 1 Select an appropriate DP tip (blue).






- 2 Fit the DP tip to the earpiece.




- 3 Fit the earpiece in the ear canal.


Step 3. Performing a test



- 1 Select a test mode using the   buttons. Select to **TEST**.




- 2 Select a stored patient or a **New** patient.

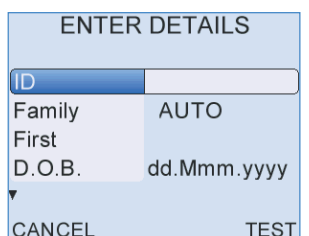


- 3 Enter patient details then select **Test**.




4 Select Right or Left ear.




5 The size of the ear being tested is indicated by the graphic. Press to **START**.

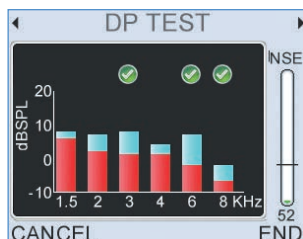


6 An OAE histogram is continuously updated during the test.



7 The test will auto-stop and a result graphic will be shown. Press the button to **REVIEW** the result.



8 The test result will be displayed at the top of the test screen. Press the button to **SAVE** the test.

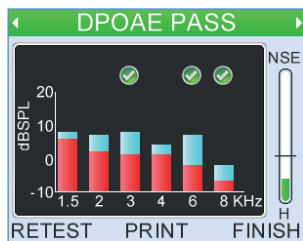

9 Press to **Retest** the same patient or to **Finish** the test.

Step 4. Disconnecting the probe



1 Unscrew the knurled sleeve.



2 Do NOT turn the main probe body.



3 Gently pull out the probe.

Step 1. Setting up your device




1 Ensure that the Otoport and the ABR module are tightly secured together.



2 Connect the OAE probe to the probe socket, aligning the 'key' and 'keyway.' Screw up the knurled sleeve until finger tight.



3 Plug the electrode connector leads into the appropriate sockets, following the colour coding. Push in firmly.



4 Press the button to switch on the Otoport. Use the and arrow buttons to navigate to the ABR screen.

Step 2. Getting ready to test



1 Prepare and clean the skin at the electrode sites to ensure low impedances. Apply electrode to high forehead.



2 Apply electrode to the nape of neck and (common) electrode to the back of the shoulder.



3 Attach , , and (common) electrodes.




4 Fit an appropriate sized tip to the probe and insert the probe in the ear to be tested. Ensure electrodes are attached correctly.

Step 3. Performing the test




1 Press the button to proceed to the Patient menu.




2 Enter patient and test details using the keypad and arrow buttons.




3 Choose the ear to be tested, or Both for a bilateral test.




4 Check impedances, total noise (TN) and powerline noise (PN) are acceptable. Reapply electrode if an impedance is marked .




5 The test will autostart if conditions are good. Press the button to manually start the test.



6 The checkfit screen shows fit size of the probe and acoustic noise (NSE). ABR will start automatically if conditions are acceptable.



7 The filling green circle represents the progress of the test towards a pass and the rising NLO bar represents the amount of data collected.



8 Use the and arrow buttons to switch between data viewing screens. To end the test, press the button. To save the test, press the button.

3.7 Using the keys and keypad

3.7.1 Control keys



The keys directly below the screen marked with a square, a diamond or a circle enable you to execute the functions offered on the screens. Their functions vary from screen to screen, but generally the right (circle) key provides affirmative options and the left (square) key provides negative options.

3.7.2 Arrow (navigation) buttons



The arrow (navigation) keys provide **Left**, **Right**, **Up** and **Down** control and allow the user to move to options available on the screen. The selected option becomes highlighted.

The left and right arrow keys scroll through the main menu options.

3.7.3

Entering characters



Character entry is similar to a mobile phone where numbered keys can be pressed sequentially to select the required character.

The order of the characters is dependent on context. For example when used to enter:

Patient ID

Numbers are presented first then capitals, e.g. 2ABC.

Family Name

For the first character capitals are presented first, then lower case then numbers, e.g. ABCabc2. For subsequent characters lower case is shown first, e.g. abcABC2.

More characters can be stored than can be displayed on the screen.

Arrows are displayed to indicate that the string continues to the left or the right. Pressing the appropriate arrow navigation keys will display the hidden characters.

3.7.4

Foreign character table



A foreign character pop-up table can be accessed by holding down the 1 button for 1.5 sec. Use the arrow keys to navigate around the table. Select **Insert** to enter the required character or select **Cancel** to close the table window.

3.7.5

Entering dates

ENTER DETAILS

ID

JUDL9700

Family

AUTO

First

D.O.B.

dd.Mmm.yyyy

CANCEL

TEST

ENTER DETAILS

ID

JUDL9700

Family

AUTO

First

06

Aug

2010

D.O.B.

07

Sep

2011

08

Oct

2012

CANCEL

INSERT

A right arrow symbol is shown at the end of a date field.

When the field is highlighted, press the right arrow key to access the calendar pop-up table. The day will be highlighted first and can be altered using the up and down arrow keys. Continue to use the left and right arrow keys to jump between the Day/Month/Year and the up and down arrow keys to select the required date.

Select **Insert** to accept the date displayed or **Cancel** to ignore the changes.

If the date has not been edited, it will remain as dd.Mmm.yyy by default.

For Date of Birth entry (**D.O.B**) the Otoport will not permit entry of a future date. **Invalid D.O.B.** will be displayed briefly at the top of the screen then the date of birth will revert to today's date. Re-edit and confirm the D.O.B. if necessary.

3.7.6

Choice bars

Left and right arrow keys are used to move through choice bar options. For example when entering patient details in the **Gender** field, pressing the right arrow key will rotate the selected option between **Not Given**, **Male**, **Female** and **Unknown**. Choice bars options are enclosed by arrow graphics.

ENTER DETAILS

Family

AUTO

First

D.O.B.

dd.Mmm.yyyy

Gender

◀ NotGiven ▶

CANCEL

TEST

3.7.7

Deleting characters



The bottom right hand key is used as a **Delete** or **Contrast** key. If the cursor is at the end of a row of characters, press this key to delete the last character.

Left and right arrow keys can be used to scroll back through the text. The selected blinking character can be replaced using the keypad data entry buttons or deleted with the delete key. Continue to press the delete key to erase characters to the right of the cursor.

3.7.8

Back light

The screen and keypad are backlit to assist in testing in dimly lit environments. The backlight stays on for 7 seconds (default) following any key press and remains on during testing. This setting can be changed in the **Configuration** area (see chapter 15).

3.7.9

Stimulus and Noise OK indicators (blue LEDs)


The two blue LEDs above the screen on the Otoport give an indication of whether stimulus and noise levels are acceptable for data collection.

The Stimulus LED is marked with an S. It is lit when the stimulus level recorded by the probe microphone is within the expected range.

The Noise OK LED is marked with an N. It is lit when the noise level recorded by the probe microphone is below the noise reject level.

3.7.10

Hard reset

In the unlikely event that the Otoport fails to respond to user control, hold the On/Off  key down for 10 seconds, in order to reset the device. You may then switch on the device as normal.

3.8

Connecting the probe to the Otoport



Prior to the testing session, connect the probe to the Otoport.


The probe plug contains a 'key' that must be aligned with the 'keyway' in the probe socket on the Otoport.




The arrow at the front of the probe plug indicates the position of the 'key' and should be aligned with the front of the Otoport.




It is possible to feel when the probe key is aligned as the probe will mate with the socket easily.

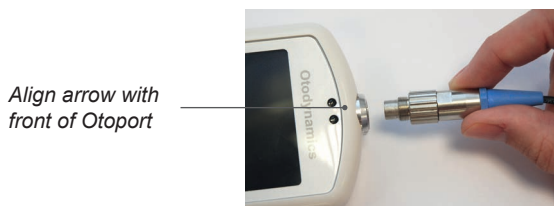

Push the probe into the socket until it hits the end stop. DO NOT force in the probe.

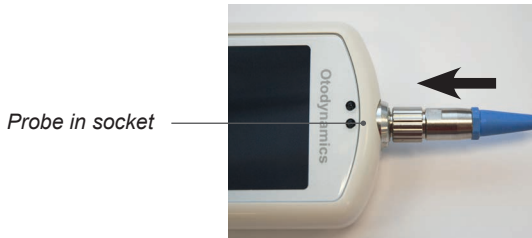


Screw up the **knurled sleeve** in a clockwise direction until finger tight.

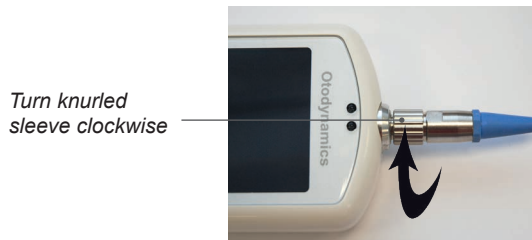


3.9

Disconnecting the probe

To disconnect the probe, unscrew the **knurled sleeve** in an anticlockwise direction until the thread is disengaged.

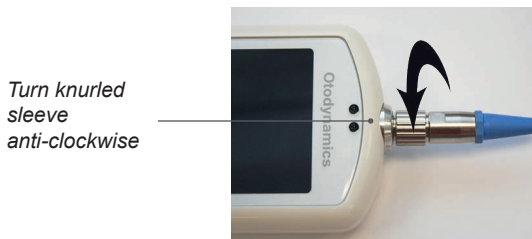


Then gently pull the probe out from the probe socket.

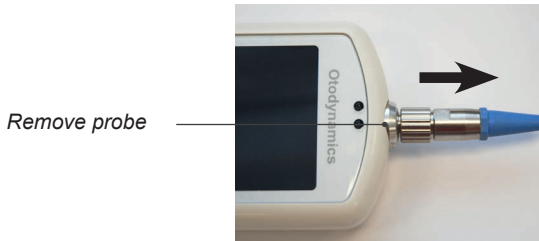

Important Note:

Do **NOT** attempt to screw or unscrew the probe by holding the main probe body (smooth chrome section).

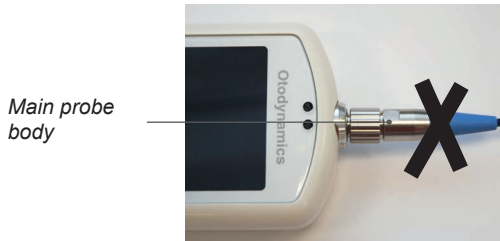


This will result in damage to the probe and will invalidate the probe warranty.

4 Switching On

4.1 Switch on screen




To switch on the Otoport press the green **On/Off power** key found at the bottom left of the keypad. The display screen will show **Switch Unit On?**.

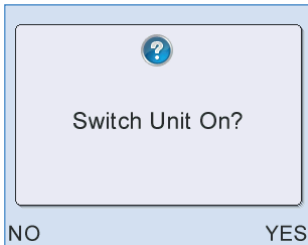

Select **Yes** to confirm Otoport switch on, or **No** to turn the unit off again. If **Yes** or **No** are not selected within two seconds of pressing on/off power key, the device will automatically turn off. The unit will turn off if any key other than **Yes** is selected. This is to prevent accidental switch on during transit.

4.2

Logo screen

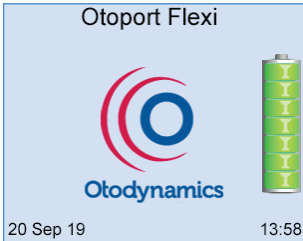


Following switch on, an Otodynamics' logo animation is displayed whilst the device performs a series of hardware system checks. In the unlikely event of any of the systems checks failing, an error message will be displayed (see section 22.5 **Hardware fault messages** for details).

A battery graphic will appear to the right of the logo to provide an indication of the **Battery Power** remaining. Please refer to chapter 21 **Otoport Power** for battery information.

A prompt will be shown if the Otoport is due to be calibrated (see chapter 25 **Calibration**).

4.3

Mode select

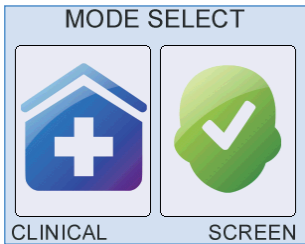

The Otoport Flexi has two distinct operating modes: **Screen** and **Clinical**.

The Screen mode is designed to run tests in the shortest possible time and to stop automatically when there is conclusive evidence that a response is present.

The Clinical mode is designed to run longer, more detailed tests that will run until the user is satisfied with the quality of the data.

Select the mode which meets your requirements.

Both modes are fully configurable and either can be disabled (see chapter 15 **Configuration**).

To return to the **Mode Select** screen, enter and then exit the **Config** area (see chapter 14 **Utilities**) or turn the Otoport off and on again.

This screen is not shown if one of the modes is disabled.

4.4

Login

Login can be enabled or disabled via the configuration menu (See chapter 15 Configuration)


If **Login** is **on** the login screen will be displayed and the user will be required to enter a name and password.

Use the left and right arrow keys to choose the correct user name from the choice bar.

Once the user is selected, use the data entry keypad to enter a corresponding **Password**, if set for that user.

To improve security during **Login**, a * symbol will replace each character as it is entered in the **Password** field. To review characters that have been entered, simply scroll back through the * using the left and right arrow keys.


When the **User** and **Password** have been chosen, select **Login** to access the device. If the **Password** has been entered incorrectly, a warning message will appear:

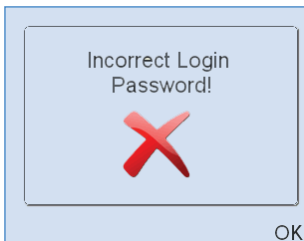

4.5




Test choice


Following the logo screen, or after successful login, the test screen for the last test used is displayed. From here you can view the **Result** for the last patient tested, edit the details for the **Last** patient tested or start a **Test** on a new patient.

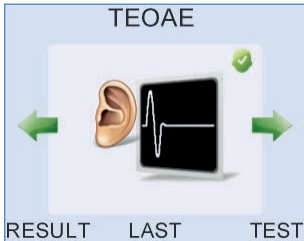


TEOAE test is an optional feature in some regions

Other module screens can be accessed using the left/right arrow keys.

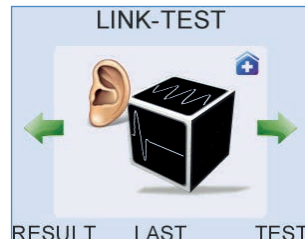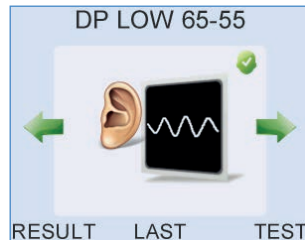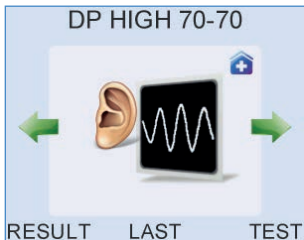


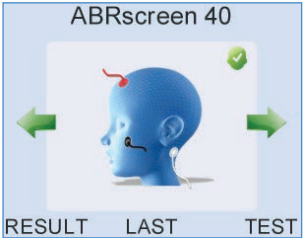

OAE+ABR model

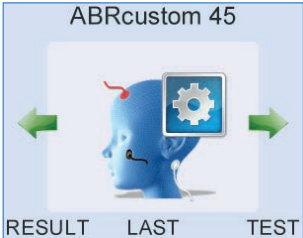

ABRcustom only available if configured
(see chapter 15)

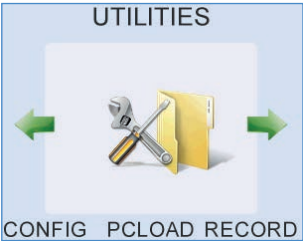

WORK LIST	
NAME	ID\NOTES
Roberts	OGPM1V02
Jones	OGPM1V03
Thomson	OGPM1V04
ADD	

See chapter 7 **Test selection** for further information on choosing a test.

5 Test preparation



Good preparation for testing will improve test results and make testing more efficient and less stressful for the baby, parents and tester.

5.1 General checks before testing

Ensure the Otoport is charged (see chapter 21 **Otoport power** for information).

Ensure the Otoport weekly checks are being regularly conducted (see chapter 17 **Quality checks** for information).

Do not run a test if there is any discharge from the ear to be tested.

Choose a quiet room, without background noises.

Ensure the patient is comfortable and settled.

Ensure you can clearly see the ear to be tested.

5.2 Environment checks for ABR

Try to minimise any interference from electrical equipment. Turn off electrical equipment and florescent lighting if possible. If equipment cannot be turned off, try to move away from it.

Ensure that all necessary disposables (sensors, tips etc) are at hand and prepared for use.

Plan where the baby will be positioned, where you will place the Otoport so it will be visible and secure and how you will route the electrode and probe cables.

5.3

Tip selection and probe fitting

Appropriate tip selection and good probe fit are essential to ensure successful OAE recordings. A good probe fit will help to block out external noise and enhance the OAE signal. The Otoport is supplied with a full range of tips to fit all ear canal sizes (see section 18.3 **DPOAE+TEOAE probe tips**). When selecting a tip, first inspect the ear to be tested to assess its size and to check that it is clear and free from debris. If debris subsequently enters the probe sound tubes, do not attempt to clean them; the coupler tubes should be changed. The correct size tip will look slightly larger than the ear canal and should fit snugly, forming a complete seal with the ear canal wall.



5.3.1

Fitting for newborns

Gently lift the pinna upwards, away from the baby's head, and then towards the back of the head. This will open the ear canal.

Insert the probe at approximately 10 o'clock (for left ear) or 2 o'clock (for right ear).

Turn the probe ear piece to 12 o'clock.

Hold the probe for several seconds. Then release the pinna and let go of the probe.



5.3.2

Fitting for newborns using ear cups

When using ear cups, there are two probe tips that you can use for the best fit of the probe to the ear cup. These are the T7M tip for TE probes and the R7M tip for DP probes; see section 18.3 for more information on probe tips.

5.3.3

Fitting for children and adults

Line up the probe to 7 o'clock (for left ear) or 5 o'clock (for right ear).

Push the probe firmly into the ear canal at this angle.

Hold the probe for several seconds. Then release the probe.

No discomfort should be felt by the patient. The weight of the probe cable should be supported to minimise the risk of the probe being pulled out during testing. Use the probe cable clip supplied, ensuring there is sufficient slack in the cable to allow for movement of the patient's head. If the correct tip is used, the probe should stay in place without aid. However, it is acceptable to hold the probe gently in the ear if the patient is restless.



5.4

Electrode fitting



5.4.1

Skin preparation

The skin at the electrode sites must be prepared to ensure that the impedance is low enough for a good recording.

Use electrode skin preparation pads/tape, exfoliating pads (e.g. Dry Prep), or a swab coated with Nuprep™ to clean each of the areas. With your thumb and finger support the skin, holding it gently taut. Swipe across the site with 3 to 4 moderately firm strokes in order to obtain a satisfactory connection to the skin. Excessive caution with skin preparation can disturb the baby more than firmer strokes.

If using a wet prep use a gauze pad to remove any residue. Avoid touching the prepared area and, to ensure that the sensor is placed directly on the prepared area, it is preferable to prepare one site at a time and immediately apply a sensor.

The use of wet gel electrodes is recommended, as the conductive gel ensures a quick and reliable low-impedance contact with the skin. However, any wired electrodes that are terminated with 1.5mm 'Touchproof' DIN 42-802 connectors may be used.

5.4.2

Placement (montage)

Electrodes are placed at three sites: the high forehead, the nape of the neck, and a reference (common) electrode on either the shoulder or cheek. In all locations avoid hair when possible. When using wet gel electrodes the sticky area around the central gel should be pressed to the skin – not the central area itself.

Shoulder (common ● black) and nape of neck (negative ⊖ white)



High forehead (positive ⊕ red)



The sensor should be placed high on the forehead near the hairline and in the centre (not offset to the left or to the right). Prepare the skin and, whilst holding the skin taut, apply the sensor.

If using snap stud electrodes, now connect the electrode cables to the sensors. Connect the red cable to the high forehead, the white cable to the nape of the neck and the black cable to the back of the shoulder.



Alternative electrode placements

The Otoport is optimised for the electrode placements described above. Alternative placements are possible, including:

		Recommended	Alternative 1	Alternative 2
Positive - Red	+	High forehead	High forehead	High forehead
Negative - White	-	Nape of neck	Nape of neck	Mastoid of test ear
Common - Black	●	Back of shoulder	Cheek	Mastoid of non-test ear

Note:

The Positive (+ Red) electrode MUST always be placed on the high forehead.

The Otoport may fail to recognise a valid ABR if an alternative place is used for the Positive (+) electrode.

6 Test troubleshooting

6.1 OAE test problems

The most frequent cause of unsuccessful OAE recordings is failure to fit the probe correctly, so that it is deep enough in the ear canal. The presence of fluid and debris in the ear canal or middle ear will also inhibit recordings.

If a pass result is not obtained, remove the probe and inspect the probe tip. Discard the tip if it has collected debris or moisture. Also check that the probe coupler tubes are clear and replace these if a blockage is noticed. Then refit the probe and try again. Problems of debris and middle ear fluid occur mostly in babies younger than 6 hours and are often cleared by feeding or turning the baby. If there is no success during the first OAE testing attempts, a second OAE testing session usually brings success when the ear has had time to clear.

Babies are best tested when they are sleeping or sleepy and successful OAE recordings are most often made one hour after a feed. The baby may settle down more easily if swaddled. Babies older than one month may be too active to test. When testing a child it can help to entertain them during the test, so they don't become too restless. Try to keep the probe cable out of their reach; using the probe cable clip may help. Instruct adults to be still and remain quiet.

Noises from the patient may not prevent successful recording, but will increase the test time. Constant environmental background noise, for example from air conditioning or machinery, may prevent a successful test. Testing should only be conducted in rooms where the noise level recording on the Otoport is mainly below the noise reject level when the probe is not fitted in the ear. Some intermittent noise can be tolerated, but constant high noise will inhibit successful recordings.

6.2

ABR test problems

6.2.1

Impedance values are too high and the test will not run

Solutions:

Wait for about two minutes. During this time the electrodes may connect better to the skin and, therefore, reduce the impedance values.

1. Check all electrode plugs are firmly inserted into the sockets of the ABR Module.
2. Press firmly onto the electrodes if impedance is only slightly high.
3. Remove and re-prepare the electrode site that has high impedance. If that fails to work, re-prepare all sites.
4. If re-prepping does not work, try a fresh set of disposable electrodes (or clean reusable electrodes).
5. 'Wet gel' electrodes, such as the Ambu Neuroline 720, can dry out especially if the foil pouch they are kept in has been opened for some time. This can result in very high impedances. Check the expiry date on the electrode pouch and then open a fresh pouch if in doubt about how long the current pouch has been open.

6.2.2

High myogenic activity/artefact reject

The most common cause of electrical interference is myogenic (muscle) activity from a restless baby.

Solutions:

1. Check that all electrode and cable connections are secure.
2. Switch off lights in the test area.
3. Do not place the Reference (Common) electrode close to the heart (front or back of the patient). Noise can be generated by a large EKG response.
4. Smooth and swaddle the baby in an effort to calm him/her. Note that electric muscle artefacts may arise from non-moving but tensed muscles (isometric contraction) – pay particular attention to the nape of the neck with this condition.

5. Touch each electrode to identify which is causing the problem, try:

- holding the skin around the electrode taut
- maintaining light pressure on the electrode
- gently stroking the baby's head
- repositioning the baby's head

6.2.3

High environment electrical noise

Audible noise in the room as well as interference from other electrical equipment may trigger an artefact reject signal.

Solutions:

1. Check that all electrode and cable connections are secure.
2. Switch off any non-essential equipment in the room.
3. Do not use mobile (cellular) phones when operating the equipment.
4. Separate the electrode cables from the probe cable if intertwined.
5. Move to a quieter location if possible.

6.2.4

No response in ear with known normal hearing

Check electrode montage (placement). Using an incorrect montage can result in very small responses, or responses that have a low template correlation.

Check probe fit. A probe that has very poor fit to the ear can result in very low stimulus levels and therefore a small or absent response.


7

Test selection








7.1




Choose test type or worklist



TEOAE test is an optional feature in some regions



unit ABR screen



ABRcustom only available if configured (see chapter 15)

Using the left and right arrow keys, choose one of the test types. The available modes will depend on whether **Screen** or **Clinical** test mode was selected.

The default **Clinical** modes are **TEOAE**, **DP High**, **DP Low** and **DP 12 Frequency**.

The default **Screen** modes are **TEOAE**, **DP Low** and **ABRscreen**.

Small icons indicate whether **Screen** or **Clinical** mode is in use. The available modes can be altered (see chapter 15 **Configuration**).

Link-Test, **Utilities** and the **Work List** are always available in both modes.

The **DP High** and **DP Low** modes allow testing at half-octave points at different stimulus levels. **DP 12 Freq** tests from 1-8kHz at quarter octave points.

Note:

Configure the modes available in the **Config** area (see chapter 15 **Configuration**). Modes turned **Off** here will not be available.

The banner at the top of the first four main menu screens shows the current test stimulus. For the DP modes, the numbers by the mode name represent the amplitude of the primary tones L1 and L2.

A test may be started from one of these screens by selecting **Last** or **Test**.

For guidance on using the **Work List**, see chapter 13.

A test may also be started from the **Patient** details screen in the **Record** area (see chapter 14).

PATIENT DETAILS	
	1/11
ID/Notes	OGPM2108
Name	Hale
D.O.B	01 Feb 2012
Gender	◀ Male ▶
BACK	PRINT TEST

You will not be able to start a test if the Otoport is connected to a PC or power supply.

7.2

Patient details

ENTER DETAILS

ID/Notes	OGPM1V00
Name	
D.O.B	dd.Mmm.yyyy
Gender	◀ NotGiven ▶
▼	
CANCEL RECORDS SAVE	

Patient details can be entered before testing by selecting **Test** (with **Quick Save Off**).

Details can also be entered after the test by selecting **Last**, this is the only route for entering details if **Quick Save** is **On**.

If you are retesting an existing patient then they can be selected, and their details viewed, from **Records** (see chapter 14).

A Date of Birth (**D.O.B**) and **Gender** may also be added for the patient.

A further three fields are available by scrolling down using the arrow keys. These are **NICU** (Yes or No), **Location** (Inpatient, Outpatient or At Home) and **Facility**.

Note:

It is only possible to store one **Facility** on the Otoport and it should not be changed for individual patients. If you wish to change the **Facility**, download and erase all test records from the Otoport first.

It is also not possible to set the **NICU** field to **Yes** if **Location** is set to **Outpatient** or **At home**. The fields are automatically corrected in this case.

If the test was run using the **Last** option, test results will be saved to the same patient. All fields except **Location**, **Facility** and **NICU** can be edited.

When the patient details are complete, select **Save**.

7.3

Select test ear



The **Select Ear** screen represents the patient facing you.


Press the right menu selection key or the right arrow key to select the **Left Ear** or press the left menu selection key or the left arrow key to select the **Right Ear**.

ABR tests may be run bilaterally (on both ears), so a third option **Both** can be chosen. Further information on bilateral ABR testing follows in chapter 10.

If the patient's previous test was saved to the same ear, the pop-up message **Last Test Saved to Left/Right Ear. Save Test to Left/Right Ear Again?** will appear. Press **Yes** to accept the current ear choice or press **No** to return to the **Select Left/Right Ear** screen.

7.4

Checkfit

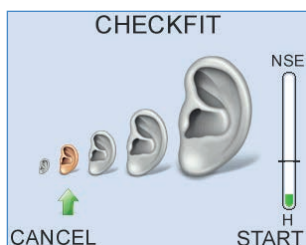

It is important to perform a test in the appropriate conditions. The **Checkfit** screen allows a user to assess the testing environment. Conditions such as high ambient noise, poor fit of the probe in the ear (including leaks) and blocked probes can be detected before starting the test.

Excessive noise or a poor probe fit may mean that the test cannot be performed or that the quality of data collected may be too low for an accurate test result to be determined.

All OAE tests begin with checkfit. ABR tests run an impedance check (see 10.1) before checkfit.

7.4.1

Fit size indicator

The **Checkfit** screen shows a Fit Size Indicator; this shows a series of ears of increasing size, indicating increasing ear canal volumes. The size of ear canal detected in Checkfit is indicated by an arrow.

During **Checkfit** the Otoport repeatedly plays a click at a fixed level and records the sound level this click produces in the ear.

The sound level recorded depends on the fit of the probe and the size of the ear canal in which the probe is inserted.

Ear canal size increases from birth to adulthood. So, given a good probe fit the sound level recorded correlates with the age of the patient.

For example, if the arrow is below the smallest ear, this indicates that the sound level recorded is that which would be expected from a small ear canal. You would expect this if you were testing a baby.

Individual ear canals vary considerably in size, so the indication of canal size can only be used as an approximate guide to probe fit.

If the position of the Fit Size Indicator corresponds with the age of the patient and **Checkfit** is displayed on the top of the screen then the probe fit and the test conditions are adequate for testing. The Stimulus and Noise OK indicators (above the screen) should also be illuminated. Select **Start** to continue the test.

If there is a disagreement between the Fit Size Indicator and the ear canal size expected of your patient, then there may be a problem with the probe or the probe fit. For example: an indication of a large ear canal in a neonate may occur if the probe has fallen out of the ear or if the probe is blocked; an indication of a small ear canal in an adult may occur because of wax blocking the canal.

7.4.2

Noise level indicator

A Noise Level Indicator is shown on the right of the **Checkfit** screen. The bar moves in response to changes in noise. For good testing conditions the bar should be consistently below the Noise Reject Level which is represented by the horizontal line across the Noise Level Indicator. The bar is filled red if the level is above the threshold and green if it is below. The threshold level is displayed numerically above the indicator. Use the up/down arrow keys to change the Noise Reject Level.

Generally higher noise reject can give faster data collection but poorer quality data. The best noise reject setting depends on both test conditions and the strength of the emission being tested. Strong emissions may be detected in a noisy environment with a high noise reject threshold. Weak emissions may only be detected in a quiet environment with a low noise reject threshold.

7.4.3

Checkfit condition information

Highlighted messages are shown when conditions are not optimum for OAE recording.

Check Probe Fit is shown if the stimulus level falls outside the accepted range.

Noisy appears if the noise level is consistently above the set noise reject threshold for a period of time.

Ringings is displayed when there is obvious oscillation within the **Stimulus Waveform** after the initial expected positive and negative peaks.


The following table describes which highlighted message will appear if more than one condition is met.

Note that highlighted messages also appear during the test.

Consistent High Noise	Stimulus Out of Range	Stimulus Ringing	Highlighted Message
No	No	No	Checkfit
Yes	No	No	Noisy
No	Yes	No	Check Probe Fit
No	No	Yes	Ringing
Yes	Yes	No	Check Probe Fit
Yes	No	Yes	Ringing
No	Yes	Yes	Check Probe Fit
Yes	Yes	Yes	Check Probe Fit

8 DPOAE test

8.1 DP stimulus calibration

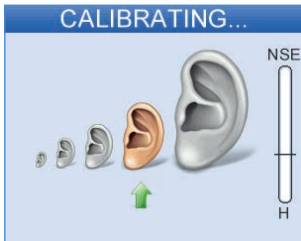

Before starting the test the Otoport will calibrate the levels of the stimulus tones which are to be used in the test. By default, this process will start automatically following **Checkfit**, or if **Start** is selected. This is necessary to account for the acoustic properties of individual patients' ear canals. If the required levels cannot be reached then the Otoport will display the message **Unable to calibrate. Check probe fit** and return to the Checkfit screen.

If calibration fails, check the probe fit and check that the probe coupler tubes are clear. Excessive noise may inhibit calibration, so ensure environmental noise levels are low. Make sure a DP (UGD - grey) probe is connected to the Otoport and not a TE (UGS - red) probe.


If calibration continues to fail, regardless of the position of the probe in the ear, it is likely that the probe has become blocked. In this case, inspect the probe coupler tubes and replace them if necessary, then run probe checks (see chapter 17) to test the probe and Otoport performance.

Following **Stimulus Calibration**, the OAE recording begins and data is collected and displayed on a choice of three test screens - an OAE histogram, a data table and an SNR progress (Circles) display. The screens are continually updated to give a real time representation of the OAE response. The left and right arrow keys can be used to toggle between the screen choices when a test is in progress. Common to all three screens is a noise level indicator to the right of the display, the title bar at the top of the screen and the **Cancel** and **End** options.

With **Neonate** mode **On**, the user is warned if the response from the probe indicates a large ear canal (see section 15.2.1).

DP test screen


The initial test screen displayed depends upon the display option set from the **Configuration** menu (see chapter 15 **Configuration**).

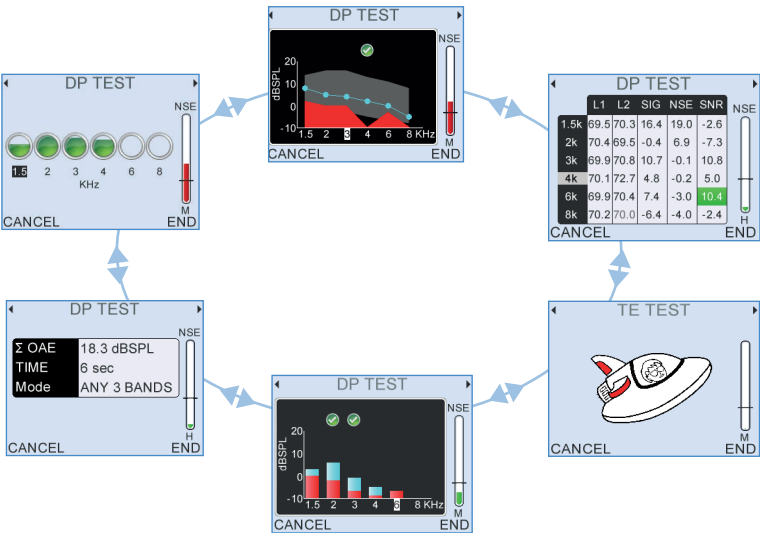

Switch between the test screens by pressing the left or right arrow keys. The Otoport will remember the last screen displayed and return to it in the next test.

8.2.1

Line and Bar graphs

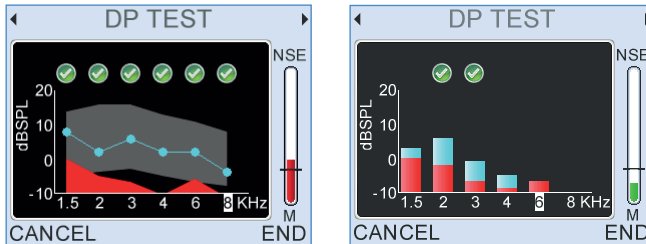

The two screens display the same test data graphically, either as a line graph or a bar graph.

The blue dots or bars at each frequency show the DPOAE signal level and the red section represents the noise level in this frequency region.

A tick/checkmark will appear above a bar/dot if the DP at that frequency has met its pass criteria. Please refer to the **Configuration** chapter for further information on the DP pass criteria.

If local **Norms** have been set in the test set up area then they will be displayed as a grey shaded area or brackets (see chapter 15 **Configuration**). Norms are for indication only and do not affect stop criteria.

The F2 frequencies are displayed below the bars/dots. The blue section of each band represents the DP signal level at the 2F2-F1 frequency and the red section represents the noise level in this frequency region.




If either the OAE signal or noise level at a DP frequency is greater than 20dB SPL, an up arrow will appear above the band to show the level is off the graphical scale.



If no data has been collected at any given frequency then no histogram will be drawn and a diamond symbol will appear instead. If at a particular frequency the environmental noise level is high during data collection, no good data will be collected at that frequency and the diamond symbol may remain for a number of loops. In constant noise the diamond may be displayed throughout the complete test.

8.2.2

Circles

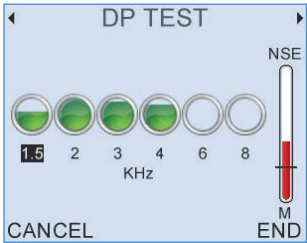


The display shows a series of small circles, each representing the SNR recorded at a particular DP frequency when the minimum signal level is met. If the minimum signal level is not met, the circle will not fill completely, even if SNR criterion has been achieved. The numbers below the circles indicate the F2 frequency in kHz. When the test has stopped, a tick/check mark is shown in the circles that passed.

The Circles display is not available in DP 12 Freq mode.

8.2.3

Infant distraction screens

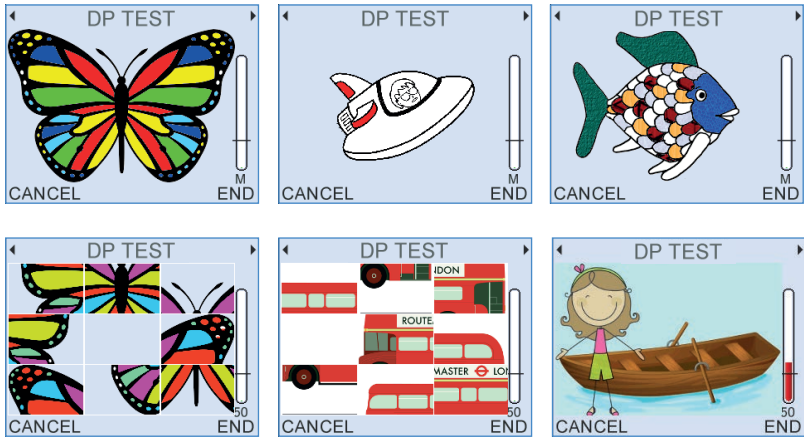

Animated infant distraction screens are available during the test. A number of alternative images are available.

Selecting the numbers on the Keypad will display the associated picture:


1 = Butterfly, 2 = Space Vehicle, 3 = Fish, 4 = Butterfly Puzzle, 5 = Bus Puzzle, 6 = Boat Picture.

These screens are designed to encourage young patients to keep still and quiet during OAE testing. They show a simple drawing that becomes more colourful if they are quiet. The quieter they are the more quickly the picture “story” progresses. If they become noisy then the colour in the picture starts to fade.

When the test is completed, the result screen will be shown as normal .

8.2.4

Data tables

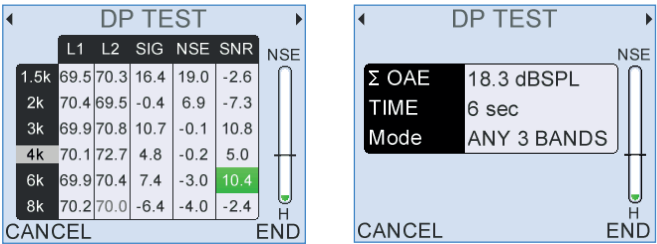

During the test the data tables can be accessed by pressing right or left arrow keys.

Data Table 1 displays the dBSPL levels of:

SIG	The signal level recorded at distortion product frequency (2F1-F2)
NSE	The average Noise level recorded at the corresponding DP frequency region (this value depends on the Noise Mode set - see chapter 15).
SNR	The Signal-to-Noise Ratio (SIG minus NSE)

A dash (-) indicates no data has been collected at that frequency.

Data Table 2 displays the current total OAE summed over the test points, the test duration and the test mode used.

8.2.5

Noise level indicator

A noise level indicator is shown on the right of screen. The bar moves in response to changes in noise. For good testing conditions the bar should be consistently below the Noise Reject Level which is represented by the horizontal line across the noise level indicator. The bar is filled red if the level is above the threshold and green if it is below. The noise level shown is calculated from the peak sound level recorded within each response window.

The letter below the indicator represents the noise reject threshold level. This can be altered using the up and down arrow keys.

The noise level indicator allows continuous monitoring of the noise level during a test.

8.2.6

Test condition information

When conditions are good for data collection **DP TEST** will be shown at the top of the screen and progress indicators will move either side of the title to show that a test is currently running. If test conditions are not optimum, a highlighted message will appear, indicating the problem. (See section 7.2.3 **Checkfit condition information**).

8.2.7

Minimum recordable signal level

Low level signals at the DPOAE frequency may not always be of cochlear origin. At each frequency the Otoport assesses the minimum recordable signal. At some higher frequencies (as listed in table below) and with stimulus levels above 65dBSPL the minimum recordable signal level increases and so a larger signal is required for a DPOAE to be recorded. If the signal level is below the minimum recordable signal level the value is disregarded and the Otoport shows a substitute 'marker' signal level of -30dB instead.

Note that reaching the Minimum valid signal level indicates only that the signal recorded is valid for processing, not that the DPOAE level that frequency is normal or that it meets the signal to noise requirement set for the test.

Below is a table of the minimum valid signal levels in dBSPL for a range of frequency and stimulus levels.

Frequency (F2 kHz)

Level (L2)	<5.2	5.6	5.9	6.1	6.4	6.7	7.0	7.3	7.6	8.0
65dBSPL	-10	-10	-10	-10	-10	-10	-10	-10	-10	-10
70dBSPL	-10	-10	-10	-7	-8	-10	-9	-8	-10	-10
75dBSPL	-10	-10	-2	-6	-7	-10	-8	-7	-7	-10

8.3

Test stop reasons

There are three possible ways in which a test can stop: AutoStop, Test Timeout and Manual End. When the test stops the data collected is assessed and a result is given as a graphic image and then written highlighted at the top of the test screen. The Otoport will beep once if a test has stopped with a DPOAE Pass result and will beep twice if the test has stopped with any other result. AutoStop and Stopping (Pass) criteria are configured in the test settings area (section 13.2).

You can pause the test by selecting **Cancel**, then select **No** to resume recording, **Checkfit** to return to the **Checkfit** stage and **Yes** to end the test.

8.3.1

Test timeout

If a test has not met the set pass criteria and the noise is consistently above the **Noise Reject Threshold Level** so that the **Maximum NLo Sweeps** cannot be achieved then the test will stop after 60 seconds, regardless of the amount of good data collected. This is to control stimulus exposure to the ear and to limit the test time to allow for reassessment of the ambient noise and of probe fit before a retest.


8.3.2

Manual end

Selecting **End** at any time will stop the test.

8.3.3

Pausing and cancelling the test

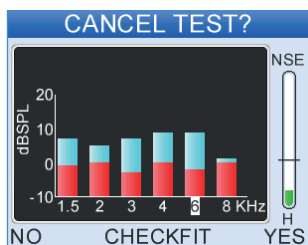







You may wish to pause a test for instance during periods of noise. When the test is paused, it is possible to cancel the test and discard the data. Select **Cancel** to pause the test. Select **Yes** to end the test and discard the data, **No** to resume the test and **Checkfit** to restart the test at the Checkfit stage.

8.4

DPOAE test results

The following table lists all possible test results with the associated results graphic and gives an explanation of the circumstances under which each result would be shown.

Test Result	Description
DPOAE Pass 	The data collected has met the criteria set. The optimum test setting will depend on your application, e.g. screening or clinical measurement (see 15.2 Test settings)
<i>Note: The following results will only occur if a DPOAE Pass is not obtained, providing test information feedback to the user</i>	
No Valid OAE 	The data collected has not met the set pass criteria and the test conditions were acceptable
Noisy 	The noisy data collected is three times greater than the low noise data collected
Poor Probe Fit 	Probe fit movement is detected that results in less than 85% of stimuli reaching calibration levels
Too Few Bands 	Insufficient bands meet their pass criteria
Stopped Too Soon 	The test has been ended manually before the required minimum amount of data has been collected

Select **Save** to skip to the **Patient Details** screen ready to **Save**.

Select **Review** to view the data of the completed test, prior to saving.

Select **Cancel** to discard the test result. A prompt requiring confirmation will be shown before the result is discarded.

9 TEOAE test

TEOAE test is an optional feature in some regions

9.1 TE stimulus adjustment



Following Checkfit, or when **START** is selected, the Otoport will attempt to adjust the stimulus level to the required level. The message **Adjusting...** is displayed while this is happening. When the correct level has been reached, the Otoport automatically begins the test.

The Otoport may not be able to adjust the stimulus to the correct level in noisy environments, if the probe fit is poor or if the patient's ear canal is unusually large. If the correct stimulus level is not reached after 10 seconds then the message **Stim out of range** will be displayed. The user then has the option to **Continue** or **Cancel** the test.

In these circumstances Otodynamics recommends that the test is cancelled. Efforts should then be made to improve the probe fit, check the probe coupler tubes are clear and improve the test environment. If adjustment continues to fail regardless of the position of the probe in the ear, it is likely that the probe has become blocked. In this case, inspect the probe coupler tubes and replace if necessary, then run probe checks (see chapter 17) to test the probe and Otoport performance. If stimulus adjustment is still unsuccessful, continuing the test may provide useful results but it is likely that the stimulus level will be incorrect. This will affect the level of OAE recorded.


With **Neonate** mode **On**, the user is warned if the response from the probe indicates a large ear canal (see chapter 15.2.3).

9.2

TEOAE test screen

The initial test screen displayed depends on the display option set from the **Configuration** menu (see chapter 15 **Configuration**).

Switch between the test screens by pressing the left or right arrow keys. The Otoport will remember the last screen displayed and return to it in the next test.

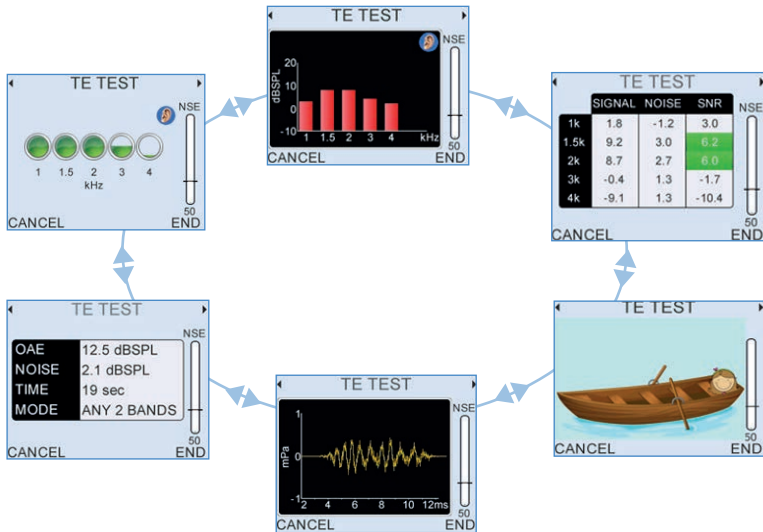


During testing the Otoport plays a series of clicks into the ear and records the response. The OAE signal is very small and difficult to distinguish from the noise made by other sounds in the room and by the patient. The longer the Otoport records for, the easier it is to distinguish the OAE signal from the noise. The Otoport looks at the ratio of the OAE signal to the noise; this is known as the Signal to Noise Ratio or SNR. The Otoport measures the SNR in a number of different frequency bands. The pass criteria are set in the **Configuration** area (see chapter 15 **Configuration**). The default pass criteria are an SNR of 6dB and a minimum signal of >5dBSPL in at least two frequency bands.

It is the responsibility of the user to ensure that the pass criteria set meet their requirements.

The test screen display depends upon the display option set from the **Configuration** menu (see chapter 15 **Configuration**). The default display is **Bars**.

9.2.1

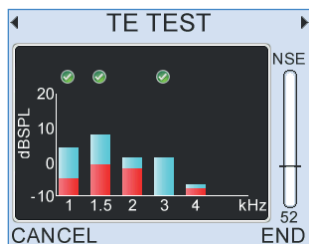


Bars



The screen displays test data graphically on the screen in $\frac{1}{2}$ octave bands: 1k, 1.5k, 2k, 3k and 4kHz. The clear section of each band represents the OAE signal level within each band and the shaded section represents the noise level at that frequency.


A tick/checkmark will appear above a bar if the band has met its pass criteria. Please refer to **Configuration** (chapter 13) for further information on the band Stop criteria.

If either the OAE signal or noise level in a $\frac{1}{2}$ octave band is greater than 20dB SPL, an up arrow will appear above the bar to show the level is off the graphical scale.

-  If either the OAE signal or noise level at a frequency band is greater than 20dB SPL, an up arrow will appear above the band to the right of the tick to show the level is off the graphical scale.
-  If no data has been collected, then a histogram will not be drawn and diamond symbols will be shown instead.
-  Brackets can be displayed to indicate normative ranges (see chapter 15 **Configuration**).

9.2.2


Circles

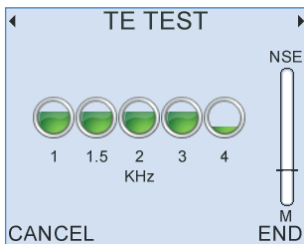

The **Circles** display shows a series of small circles. Each small circle represents the SNR recorded in a particular $\frac{1}{2}$ octave frequency band when the minimum signal level is met. If the minimum signal level is not met, the circle will not fill completely, even if SNR criterion has been achieved. The numbers below the circles indicate the kHz frequency of the centre of the $\frac{1}{2}$ octave band. When the test has stopped, a tick/check mark is shown in the circles that passed.

If the test mode is set to **Wideband** or **Narrow** (see **Configuration**, chapter 15), only one circle is shown. A fuller circle indicates that the SNR and signal level are closer to the pass criteria. When the test has stopped, a tick/check mark is shown in the circle if the test has passed.

9.2.3 Infant distraction screens

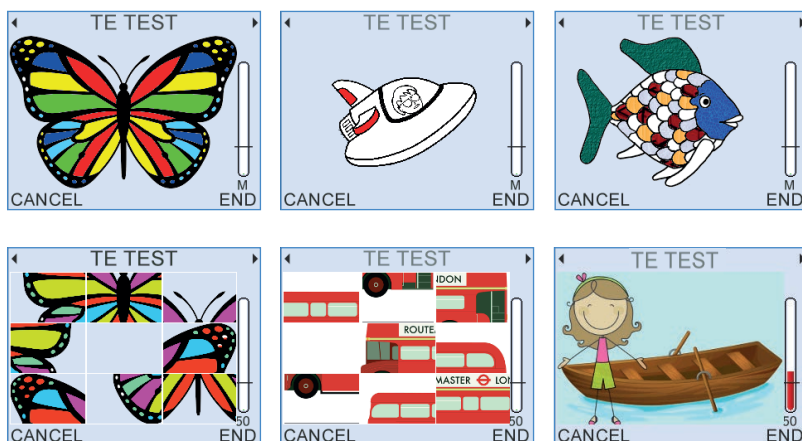

Animated infant distraction screens are available during the test. A number of alternative images are available.

Selecting the numbers on the Keypad will display the associated picture:


1 = Butterfly, 2 = Space Vehicle, 3 = Fish, 4 = Butterfly Puzzle, 5 = Bus Puzzle, 6 = Boat Picture.

These screens are designed to encourage young patients to keep still and quiet during OAE testing. They show a simple drawing that becomes more colourful if they are quiet. The quieter they are the more quickly the picture “story” progresses. If they become noisy then the colour in the picture starts to fade.

When the test is completed, the result screen will be shown as normal.

9.2.4


Response waveform

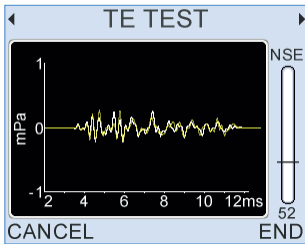

The response waveform screen displays the two interleaved OAE waveforms (named A and B). Waveform A is shown in orange and waveform B in yellow. Waveforms that correlate well represent good quality recordings with low noise. Significantly different waveforms indicate a noisy recording. As the test continues the noise levels will be reduced by averaging and the two waveforms will show better agreement. Examining the waveforms can help troubleshoot testing problems. Typical TEOAE response waveforms have energy distributed across the response window with the higher frequencies appearing early in the response window and low frequencies later. Waveforms dominated by a single frequency may be the product of strong spontaneous OAEs. Waveforms dominated by a single frequency which decays rapidly may be due to a faulty probe or a ringing stimulus. If you are concerned about the performance of your Otoport, run the system QA tests (see chapter 17 **Quality tests**).

9.2.5

Data tables

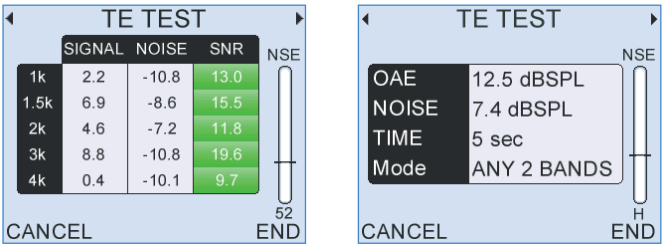

Two data tables may be accessed during the test by pressing right or left arrow keys.

The first data table displays the dB levels at the specified half octave frequencies.

Signal	The signal level recorded in dB SPL
Noise	The Noise levels recorded in dB SPL
SNR	The Signal-to-Noise Ratio (SIGNAL minus NOISE dB) ; a dash (-) indicates no data has been collected at that frequency

The second data table displays the current total OAE, the total noise, the test duration and the current test mode. It can be accessed during the test by pressing right or left arrow keys.

9.2.6

Noise level indicator

A Noise Level Indicator is shown on the right of the **Checkfit** screen. The bar moves in response to changes in noise. For good testing conditions the bar should be consistently below the Noise Reject Level, which is represented by the horizontal line across the Noise Level Indicator. The bar is filled red if the level is above the threshold and green if it is below. The noise level shown is calculated from the peak sound level recorded within each response window.

The letter below the indicator represents the noise reject threshold level. This can be altered using the up and down arrow keys.

The noise level indicator allows continuous monitoring of the noise level during a test.

9.2.7 Test condition information

When conditions are good for data collection **TE TEST** will be shown at the top of the screen and progress indicators will move either side of the title to show that a test is currently running. If test conditions are not optimum, a highlighted message is shown to indicate the problem. (See 7.2.3 **Checkfit condition information**).

9.3 Test stop reasons

There are four possible ways in which a test can stop: **AutoStop**, **Maximum NLo Sweeps**, **Test Timeout** and **Manual End**. When the test stops the data collected is assessed and a result is given as a pop-up graphic, then as a highlighted message at the top of the test screen. The Otoport will beep once if a test has stopped with a **TEOAE Pass** result and will beep twice if the test has stopped with any other result.

9.3.1 AutoStop

If the test data collected meets the set pass criteria then the test will AutoStop and a large checkmark will be displayed.

9.3.2 Maximum number of NLo sweeps

If a test has not met the set pass criteria it will stop when the **Maximum NLo Sweeps** (recordings made with a noise level below the rejection threshold) is reached. This is a representation of the amount of good data sweeps required before a **No valid OAE** result can be given.

9.3.3 Test timeout

If a test has not met the set pass criteria and the noise is consistently above the **Noise Reject Threshold Level** so that the **Maximum NLo Sweeps** cannot be achieved then the test will stop after 300 seconds, regardless of the amount of good data collected. This is to control stimulus exposure to the ear and to limit the test time to allow for reassessment of the ambient noise and of probe fit before a retest.


9.3.4 Manual end

Selecting **End** at any time will stop the test.

9.3.5

Pausing and cancelling the test





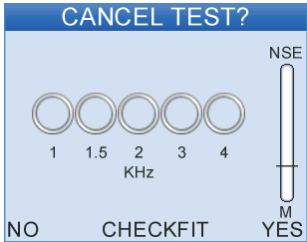

You may wish to pause a test for instance during periods of noise. When the test is paused, it is possible to cancel the test and discard the data. Select **Cancel** to pause the test. Select **Yes** to end the test and discard the data. Select **No** to resume the test and **Checkfit** to restart the test at the Checkfit stage.



9.4

TEOAE test results

The following table lists all possible test results with the associated result graphic and gives an explanation of the circumstances under which each result would be shown.

Test Result	Description
TEOAE Pass 	The data collected has met the criteria set. The optimum test setting will depend on your application, e.g. screening or clinical measurement (see 15.2 Test settings)
<i>Note: The following results will only occur if a TEOAE Pass is not obtained, providing test information feedback to the user</i>	
No Valid OAE 	The data collected has not met the set pass criteria and the test conditions were acceptable
Noisy 	The noisy data collected is three times greater than the low noise data collected
Poor Probe Fit 	Probe movement has been detected
Too Few Bands 	Insufficient bands meet their pass criteria
Stopped Too Soon 	The test was ended manually before the required minimum amount of data has been collected

Select **Save** to skip to the **Patient Details** screen ready to **Save**.

Select **Review** to view the data of the completed test, prior to saving.


Select **Cancel** to discard the test result. A prompt requiring confirmation will be shown before the result is discarded.

10 ABR test

The ABR test is only available on Otoport OAE+ABR products



Use the left or right arrow key to choose your ABR test screen.

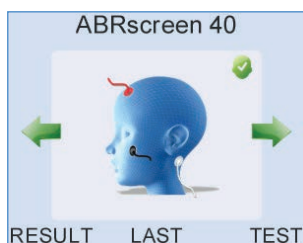

Note:

The ABR test can operate in different Modes. The following text refers to Screening Mode, where Autostart is ON. See section 15.2.9 in the **Configuration** chapter for Mode configuration option. The electrode colours are for the standard electrode connection cable and may differ if other cables are in use.

Connect the electrode leads and the OAE probe to the ABR unit and prepare your patient. Connect the red (+ve) cable to the high forehead, the white (-ve) cable to the nape of the neck and the black (common) cable to the back of the shoulder (see chapter 5 **Test preparation** for full details).

Select **Test** to begin testing.

Note:


If you see the message “ABR Mains is Not Set”, your Otoport has not yet been permanently configured for your region. You must select the powerline frequency in your region (see **ABR Mains** in 15.2) Test Settings).

10.1

Impedance check

The Otoport checks the quality of the connection between the skin and each of the three electrodes. This takes 2-3 seconds. A low impedance provides a good connection. Achieving optimum electrode impedance requires practice and experience.

The Otoport also checks the noise levels, marked TN and PN on the screen.

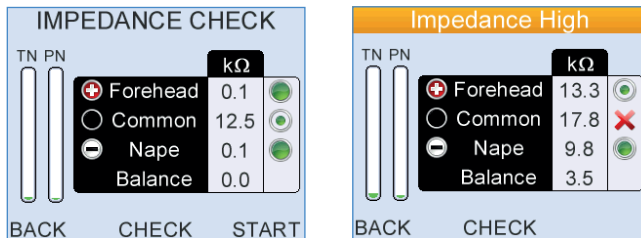

Good test conditions are necessary for efficient testing. Test conditions depend on electrode impedance and noise levels. The Otoport automatically decides if the test conditions are good, moderately good or poor:

If test conditions are good

The ABR test will start automatically if the electrode impedances are good and the electrical noise (EEG) is low for a few moments.

If test conditions are moderately good

If test conditions are moderately good they are satisfactory for testing, but could be improved; the test will not start automatically. You have two alternatives: you may manually begin the test by selecting **Start**; or try to improve the test conditions (for example by reapplying the electrodes or by settling the baby or by reducing the noise).

Observe the symbols next to each electrode on the screen. Green circles indicate the quality of the electrode connection. The more the green circle is filled the better the connection.

If you refit any electrodes then you must select **Check** to re-measure the impedances.

If the test still does not start automatically, observe the two noise bars TN (EEG Noise), and PN (Powerline Noise). They may be high. For advice on how to reduce the noise see section 6.2 **ABR test problems**.

The test will start automatically when conditions are good.

If you are unable to improve test conditions then you may manually begin the test by selecting **Start**.

If test conditions are poor

If impedance or noise conditions are poor then the test will not start and it will not be possible to start a test manually. A message on the screen will show the problem. It will tell you if EEG Noise, Powerline Noise or Impedance are preventing the test from starting. Try to resolve the issue so that testing can start.

- If any electrode impedance is marked with X then refit that electrode
- If High EEG Noise is shown then try to settle the baby.
- If High Powerline Noise is shown and electrode impedances are good, then see if there is any electrical equipment in the room that can be turned off.

(See section 6.2 **ABR test problems** for more detail).

Select **Back** to cancel the test.

If required, further advice on electrical noise indicators and impedance assessment levels is provided on the next two pages.

Further advice on ...





Otoport impedance measurements

The impedance of each electrode, Forehead (+ve), Nape (-ve) and Common are shown in the Impedance Check panel.

Green circles are displayed for all impedance values where testing is possible.

The larger the green circle, the better the electrode connection (i.e. the lower the impedance). A red cross is shown at levels where impedance is poor and testing is not possible.

The ranges for each symbol displayed are:

- Less than 4 k Ω : Optimum ()
- 4 k Ω to 12k Ω : Good ()
- 12 k Ω to 16k Ω : Moderate ()
- More than 16 k Ω : Poor ()

The green LED lights on the top of the ABR unit will be lit if the connection of the electrode closest to that light is optimum, good or moderate. Autostart requires that all impedances are optimum or good.

The Balance result indicates the difference in the skin impedance between the Nape and Forehead electrodes. Balances higher than 12 k Ω are Poor (X) and will prevent the test from starting.

If the impedance values are too high refer to 6.2 **ABR test problems**.

Note that testing is possible on the Otoport with moderate electrode impedances if there is sufficient balance between the electrodes and the powerline interference is low. This is decided automatically by the Otoport.

Select **Check** to re-run the impedance check.

Further advice on ...

Electrical noise indicators

The bars on the left of the screen indicate the electrical noise levels. The lower the test noise the more rapidly an ABR response will be detected.

Electrical noise has multiple sources:

- Interference from other electrical devices (mains/powerline noise)
- Noise from muscle activity (myogenic noise)
- Noise from brain activity (EEG)

The right hand bar (labelled PN) estimates the level of noise from electrical wiring and other devices. This level is high if there is a lot of interference from electrical noise and/or one or more of the electrodes is poorly connected (has high impedance). If impedance levels are acceptable but the PN noise level remains high try:

- Turning off or moving other electrical appliances (including lights)
- Moving to a different test location

The left hand bar (labelled TN) estimates the total level of noise from everything except other electrical devices. If this level is high it is likely that the patient is moving or is not relaxed. Try to settle the subject and ensure that the neck is supported and muscles are relaxed.

If either level remains high refer to 6.2 **ABR test problems**.

10.2

Checkfit



The test stimulus in ABR tests can be provided either by inserting the probe into the ear, as for OAE testing, or by applying an ear cup to the ear and inserting the probe into the ear cup. Ear cups can be particularly useful in neonates with very small ear canals where a secure probe fit is not possible. They can also be useful in preventing the probe from being dislodged by movement during testing.

If ear cups are not in use then Checkfit proceeds as for OAE tests (see section 7.2 for details).

Checkfit with ear cups is described below.

10.3

Ear cup Checkfit

To test with ear cups, the **Ear Cup** mode in **ABR Other Settings** must be set to **Auto** or **On**. The T7M tip (UGS probes) or the R7M tip (UGD probes) should be used to secure the probe to the ear cup. See section 15.2.9 for more details.


Ear Cup mode set to Auto

In Checkfit, the device will check whether ear cups are being used by checking if a large cavity has been detected. If this is the case, then the user will be prompted with a message to confirm. There will be three options: **Yes**, **No** and **Checkfit**. Using the probe direct in a neonate ear will always create a small cavity, but using large (adult) ears may trigger the prompt.

If **No** is selected, the device will go into normal Checkfit.

If **Checkfit** is selected, the device will go back into Checkfit and re-check whether ear cups are being used or not.

If **Yes** is selected, the device will go into ear cup Checkfit as shown below.

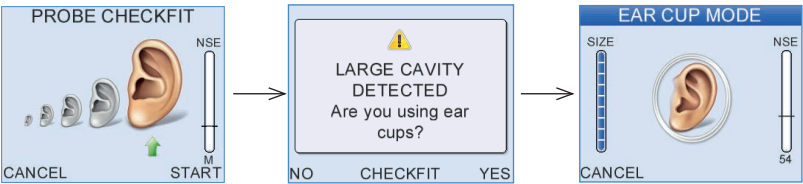

Ear Cup mode set to On

The device will go straight to ear cup Checkfit without checking for ear cup use.


Ear Cup mode set to Off

The device will go straight to normal Checkfit without checking for ear cup use.

ABR test

During the test the Otoport plays a series of clicks into the ear and records the electrical response from the sensors (electrodes). The ABR signal is very small and difficult to distinguish from other electrical signals.

The ABR test screen shows progress towards the detection of an ABR response.

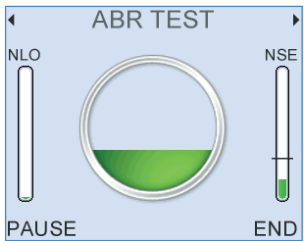

The circle indicates the probability that an ABR response is present. The circle is filled when there is 99% confidence that a response is present.

NLO is an indication of the amount of data which has been collected with the noise lower than the noise reject level.


The test will end automatically when either the circle is filled (there is a ABR response present), when the blue NLO bar is filled (a full set of data has been recorded but no response has been detected), or when test noise (ABR noise) has become so low that any valid ABR would already have been detected and so further testing is redundant.

NSE is an indication of the amplitude of the current electrical noise level. The lower this value is, the faster the test will be. The data measured during this time will be ignored. If there is high noise for a consistent period then an impedance test is automatically run and the message 'Checking Impedance' will be displayed. If impedance levels have worsened significantly since the start of the test then the test will be automatically paused.

Pressing the left and right arrow keys displays the **Data Summary** and **Waveform Display** screens.

10.4.1

Data summary

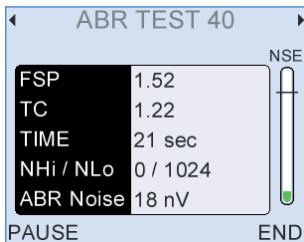

Fsp

The Fsp is a measure of the likelihood that a response is present (see *Eberling C., Don M. Scand Audiol 1984;13:187-197*).

TC

Template correlation (TC) is a measure of the similarity of the current waveform to a template constructed from the responses of 30 neonates aged 0 to 6 weeks.

Time

Shows the duration of the test.

NHi/NLo

NLo shows the number of sweeps accepted into the average. NHi shows the number of sweeps rejected due to high electrical noise levels.

Accepted

Shows the number of sweeps accepted into the average.

Rejected

Shows the number of sweeps rejected due to high electrical noise levels.

ABR Noise


Shows the estimate of residual noise in the averaged response that is used in the Fsp calculation.

If the signal which has been recorded is very small ($<15\text{nV}$), and no sign of an ABR has been detected, the test will stop automatically with a 'No Valid ABR' result as continuing the test would not find an ABR present.

If ABR noise is too high ($>85\text{nV}$), a valid ABR cannot be detected, so the test will continue to run even if other pass criteria are met.

10.4.2

Waveform display

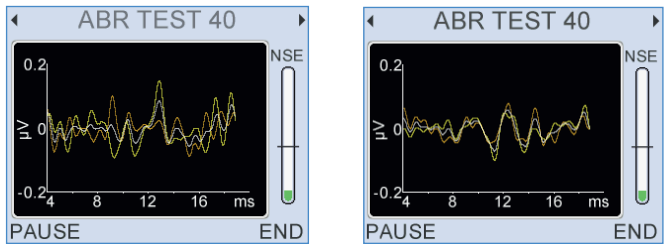

Noisy ABR

Good ABR

This screen shows the averaged ABR waveforms collected. Two waveforms are collected from interleaved averages so that the correlation between the two can be assessed. Close agreement between the waveforms indicates that a clear response is present (right), disagreement between them shows the presence of noise (left). Excess noise may obscure an ABR. The alternative waveforms are displayed in orange and yellow. The average of these two waveforms is shown in white.

The Fsp and template correlation (TC) measures are based on the final average (the white line), not on the subaverages.

10.4.3


Impedance monitoring

During the test, if progress towards ABR detection is slow, the impedance levels are automatically checked in the background.

- If impedances are low, the test will continue.
- If impedances are high, the test is paused and the 'Impedance Check' screen will be displayed.

10.4.4

Stimulus monitoring

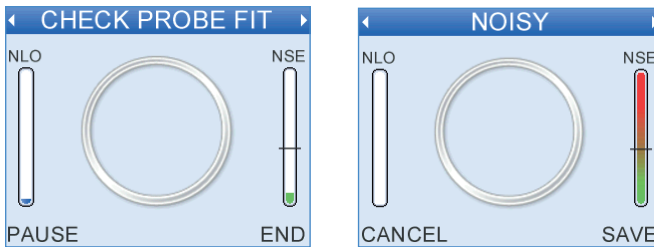

At intervals during the testing the acoustic stimulus and noise levels are checked. If the stimulus level has changed the 'Check Probe Fit' message is shown. If the environment has become too noisy to test the 'Noisy' message is shown. In either case data collection is suspended until stimulus and noise levels are within range again. The Otoport will beep to warn the user if test conditions of either 'Check Probe Fit' or 'Noisy' conditions are present for too long.

If the 'Check probe fit' message is shown, it is most likely because the probe has fallen out of the ear. Adjust the probe fit until the message goes away; data collection will automatically restart.

10.4.5

Pausing the test

Select **Pause** to temporarily stop data collection. You may wish to do this if the test environment worsens (for example the subject becomes temporarily active, an electrode becomes detached or the probe falls out of the ear). If a test is paused an impedance check is automatically run and electrical noise is monitored (as in section 8.1).

Failure to measure discernible ABR data within the defined test time, and within acceptable NLO range or before ABR noise target is reached, will return a **No Valid ABR** result.

10.4.6

Test stop reasons




There are five possible ways in which a test can stop, described below. When the test stops the data collected is assessed. The result is given as a pop-up graphic and written highlighted at the top of the test screen. The Otoport will beep once if a test has stopped with an ABR Pass result and will beep twice if the test has stopped with any other result.

AutoStop

If the test data collected meets the set pass criteria then the test will AutoStop and a large checkmark will be displayed.



The test result can be saved at this point, or the results can be reviewed prior to saving. If **Review** is selected, three screens are available by using the left and right arrow keys.

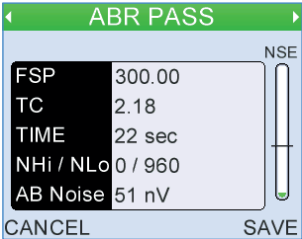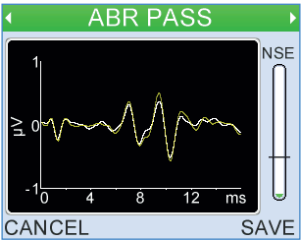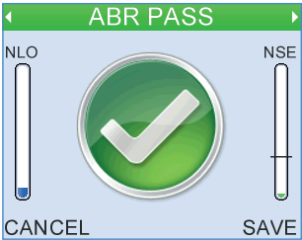

Test timeout

If a test has not met the set pass criteria then the test will stop after 10240 sweeps have been collected, or after 10 minutes.

Noise target reached

If the residual noise in the averaged test (ABR Noise) becomes so low that any ABR present would already have been detected, then further testing is redundant, so the test is ended.

Probe fit lost or high acoustic noise

If the 'Check Probe Fit' or 'Noisy' messages (see 10.3.3) are displayed for an extended period, the test will automatically stop.




Manual end

Selecting **End** at any time will stop the test.

10.4.7

Test results

The following table lists all possible test results with the associated result graphic and gives an explanation of the circumstances under which each result would be shown.

Test Result	Description
ABR Pass 	The data collected has met the pass criteria. A clear ABR has been found. Note: Optimum pass criteria will depend on your application, e.g. screening or clinical measurement (see 10.3 Test settings).
No Valid ABR 	The data collected has not met the set pass criteria and the test conditions were acceptable. In infant screening, this result supports referral for audiological investigation.
Noisy 	There was too much acoustic noise to test. The 'Noisy' message would have been displayed during testing (see 7.3.4).

Poor Probe Fit




The last stimulus level recorded changed from that recorded at the start of the test by $>3\text{dB}$, or the last acoustic noise level recorded was high.

Stopped Too Soon



The test has been ended manually before the minimum amount of data required had been collected.

Atypical Waveform



The template correlation (TC) is low but Fsp is high. A possible ABR has been detected but it did not match the neonate template. This might occur if an adult were tested or if electrodes were incorrectly connected or reversed. (Only obtained with pass criteria PC2 and PC3).

High Mains Noise




Interference from electrical equipment prevented the test from passing. The Fsp pass threshold was elevated due to this interference and the Fsp did not reach this higher threshold.

High Impedance



The electrode impedances measured at the end of the test were high and may have prevented an ABR from being recorded. This could be caused by electrodes becoming disconnected from the patient during testing.

High EEG Noise



Electrical noise during the test prevented an ABR from being recorded. This occurs when the noise recorded is too high (above 40nV) at the end of the test. This is most likely caused by the baby being unsettled during the test (myogenic interference).

After the test end, ABR test results are saved.

10.5

Bilateral ABR testing





Bilateral ABR tests automatically run tests on both ears in sequence, right ear then left ear. Ear cups are recommended for bilateral testing and both ears should be prepared before testing commences. The current test ear is indicated during the test by a blue or red icon on the test screen.

Checkfit and Test


Right ear




Left ear

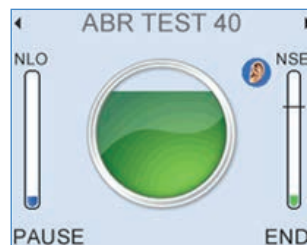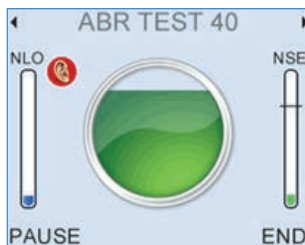

When the right ear is completed the test result will be displayed briefly before testing on the opposite ear starts.

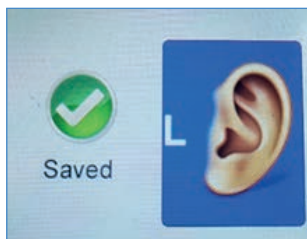

When both tests are complete, stop reason icons for both ears will be shown on the screen together.

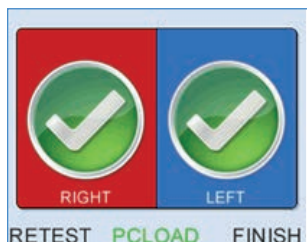

It is not possible to review bilateral ABR tests in detail at the end of test. If you wish to review the tests select the **History of Last** option from the patient menu (see chapter 8 **Patient details**).

This is an optional feature in some regions.


11 Saving the test



11.1 Quick Save option

The options available from the test result screen depend on the **Quick Save** option (see chapter 15 **Configuration**)


11.1.1 Quick Save Off

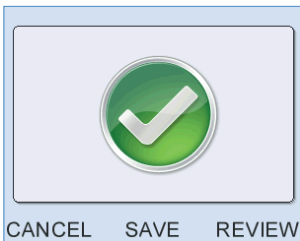

If **Quick Save** is **Off**, select **Save** to **Save** the test result.

Select **Cancel** to discard the test result. A prompt requiring confirmation will be shown before the result is discarded.


Select **Review** to view the data of the completed test, prior to saving.

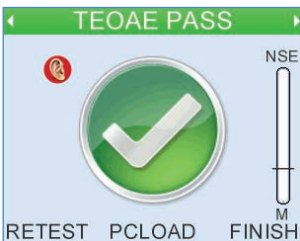

Select **Retest** to save the result and run another test on the same patient. This will navigate back to the ear selection screen to select the test ear for the next test.

Select **PC Load** or **Print** (the option available will depend on your setup (see 15.4.4) to send the test result to the Otoport printer or to the PC.

11.1.2 Quick Save On

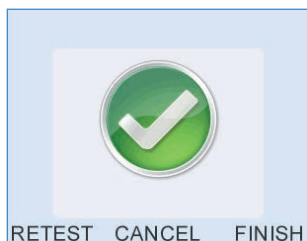

If **Quick Save** is **On**, the options after test are **Retest**, **Cancel** and **Finish**.

Select **Cancel** to discard the test result. A prompt requiring confirmation will be shown before the result is discarded.

Select **Retest** to save the result and run another test on the same patient. This will navigate back to the ear selection screen to select the test ear for the next test.

Select **Finish** to return to the main menu.

Unless **Cancel** is selected the test will be saved to the current patient or will be given an automatic ID and name. This name and ID may be edited by selecting **Last** from the main menu screen. If **Automatic print** is selected (see chapter 15 **Configuration**), the print routine will be activated at this stage. After printing or immediately after saving, the unit will return to the **Main Menu**.

11.2

Patient details

ENTER DETAILS	
ID/Notes	OGPM1V00
Name	
D.O.B	dd.Mmm.yyyy
Gender	◀ NotGiven ▶
<div> CANCEL RECORDS SAVE </div>	

The **Enter details** screen is displayed. The patient **ID** is filled with an automatically generated ID. If an ID is not required, this field may be used to enter notes. The **Name** field displays **Auto**. The user may save these details or overwrite them with alternative patient details.

A Date of Birth (**D.O.B**) and **Gender** may also be added for the patient.

A further three fields are available by scrolling down using the arrow keys. These are **NICU** (Yes or No), **Location** (Inpatient, Outpatient or At Home) and **Facility**.

Note:

It is only possible to store one **Facility** on the Otoport and it should not be changed for individual patients. If you wish to change the **Facility**, download and erase all test records from the Otoport first.

It is also not possible to set the **NICU** field to **Yes** if **Location** is set to **Outpatient** or **At home**. The fields are automatically corrected in this case.


Alternatively, the user may select **Records** and choose an existing patient record to which the current results may be appended.

If the test was run using the **Last** option, test results will be saved to the same patient. All fields except **Location**, **Facility** and **NICU** can be edited.

When the patient details are entered, select **Save** to store the result.

11.3

Review

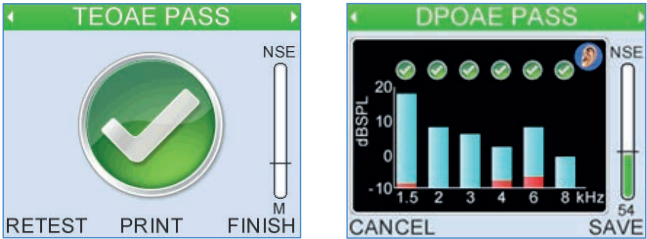


After **Saving** the user is given the option to **Print** the test results, to **Retest** the same patient or to **Finish** and return to the main menu.

Retest will start a new test of the same type for the patient. This can be used to retest the same ear or to test the opposite ear.

Print will print the current test result (default) or all the test results for the current patient (see section 15.4.4 **Setup**).

11.4

Last



After one ear has been tested, further tests can be added to the same patient record by selecting **Last** from the main menu. Patient details can be amended and tests printed using this function.

From the **Main Menu** select **Last**. The **Patient Details** screen is displayed.

PATIENT DETAILS	
1/1	
ID/Notes	OGPM1V00
Name	Brown
D.O.B	05 Jan 2012
Gender	◀ Female ▶
<div> BACK PRINT TEST </div>	

Select **Test** to start a new test with the patient details displayed. Select **Print** to print all tests saved to this patient, or select **Back** to return to the main menu.

The details stored can be edited by using the up/down buttons to locate the correct field and then entering the new data using the keypad. All fields except **Location**, **Facility** and **NICU** can be edited. When an edit has been made the screen will change:

ENTER DETAILS

ID/Notes	
Name	Brown
D.O.B	05 Jan 2012
Gender	◀ Female ▶
CANCEL	
SAVE	

If you are happy with the changes you have made select **Save**. To discard the changes select **Cancel**. Once changes are saved or cancelled the initial menu options return (**Back**, **Print** or **Test**).



11.5

Result




Select **Result** to review the tests results for the current patient.


Select displays the detailed result for this test. Select **Print** to print this test result.

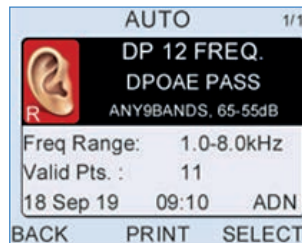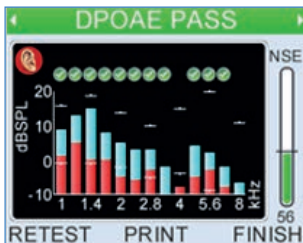

ABR test summary screen

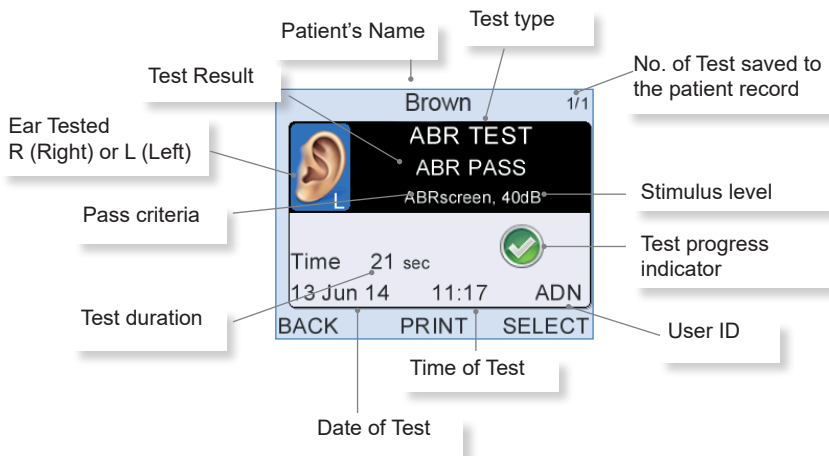

12 Link-Test

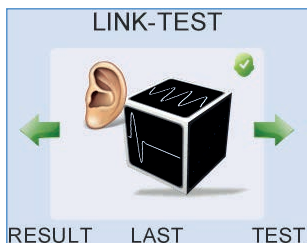

The **Link-Test** function allows a sequence of tests to be run automatically. It can be used to run all the tests currently available on the same ear (i.e. if all modes are set in **Config** as **On**, then it will run a TE, then a DP High, then a DP Low. If any mode is turned **Off** in **Config** (see section 15.2 **Test Settings**) then that mode will not be included in Link-Test. If only one test mode is switched on, then **Link-Test** is not available.

Select **Link-Test** from the scrolling modules.

Enter **Patient Details** and select the test ear.

The first test in the sequence will then begin. The test will run as it would if it had been started from the TE or DP Test menus (chapters 8 and 9) except that all tests will auto-start, regardless of the setting in **Config**. When one test has finished the Otoport will proceed to the next without any action from the user.

The result of the last test performed is available for review at the end of the sequence. The other results can be reviewed in **Records**.

13 Work List

The **Work List** allows details for multiple patients to be entered into the Otoport prior to testing. This eliminates the need for data entry while with the patient, enabling faster, more flexible testing. To use the Work List, it must be turned on in the **Config** area (see chapter 15).

Access the **Work List** by using the left or right navigation keys from the main menu.

If there are patients in the Worklist, then the Worklist will be the first screen shown when the Otoport is switched on. This aids efficient testing of the loaded patients.

13.1

Adding Patients

WORK LIST	
NAME	ID\NOTES
Roberts	OGPM1V02
Jones	OGPM1V03
Thomson	OGPM1V04
ADD	

If the Work List already contains patients scroll down to the last line which will be empty then select **Add**.

Complete the required details on the **Patient Details** screen. The **ID/Notes** and **Name** fields are pre-filled but can be over-written.

PATIENT DETAILS

ID/Notes

OGPM2100

Name

Brooks

D.O.B

01 Feb 2012

Gender

Male

BACK

SAVE

TEST

When details are complete select **Save** to save the details to the Work List, **Test** to run a test on this patient immediately or **Back** to discard these patient details.

Up to 50 patients may be added to the worklist.

Editing details

Scroll to the required patient. Select **Details** to edit the patient information on the **Patient Details** screen.

13.3

Deleting Patients

Scroll to the required patient. Select **Delete** to remove the patient from the Work List.




Select **Yes** to confirm the deletion of the selected patient from the Work List. Select **All** to delete all of the patients from the Work List. Select **No** to return to the Work List without deleting any patient details.

13.4

Testing from the Work List

Scroll to the required patient and select **Test**.

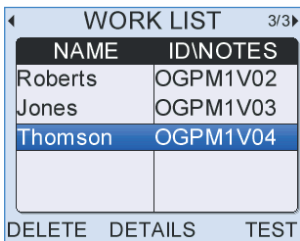


Use the left and right arrow to scroll through the stimulus options. Select **Test** on the required screen to begin testing this patient.

See previous chapters for information on performing the different tests.

When a test has been saved to a patient the patient details are removed from the Work List.

14 Utilities

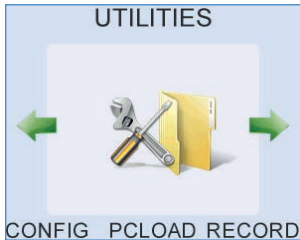

Select **Record** to see the **Result** of previous tests and to view the details of patients previously tested.

Record also allows the user to select a previously tested patient for a new **test**.

Records may only be deleted from within the **Configuration** area, via the **System** menu, from the **Memory Status** screen (see chapter 15).

Selecting **Record** presents the user with the list of patients tested.

Select **Config** to change configuration settings (see chapter 15).

14.1

Patients tested

PATIENT 1/11	
NAME	ID/NOTES
Hale	OGPM2108
Morris	OGPM2107
Anders	OGPM2106
Peterson	OGPM2105
▼Woods	OGPM2103
BACK	DETAIL RESULT

The **Patient** list displays the **Name** and **ID/Notes** field for each patient. The Up and Down arrow indicators to the left show that there are other patient records not currently visible on screen. At the top of the screen, the total number of patients in the list and the position of the selected patient are displayed: 226/234 indicates that the highlighted patient is 226th in a list of 234 patients.

Use the up and down arrow keys to scroll through the list one **Patient Record** at a time. A selected patient will be shown as highlighted in the list.

Use the left and right arrow keys to skip through the **Patient** list ± 5 records at a time.

Select **Detail** to review the **Patient Details** of the highlighted patient or to run a new **test** on this patient.

Select **Result** when a patient is highlighted to inspect the patient's saved **Test Results**. A summary of each test will be shown.

Select **Back** at any time to exit the **Patient** list screen and return to the test screen.

14.2

Patient details

PATIENT DETAILS

1/11

ID/Notes	OGPM2108
Name	Hale
D.O.B	01 Feb 2012
Gender	◀ Male ▶

BACK

PRINT

TEST

The **Patient Details** screen allows the user to see the **ID/Notes**, **Name**, Date of Birth (**DOB**) and **Gender** stored for a particular patient.

Selecting **Test** from this screen starts a new test, the result of which will be saved with the records of the selected patient.

Selecting the up and down arrows on the patient details screen displays the patients before or after the current patient in the patient list. Selecting the left and right arrows displays the test results for the selected patient.

Select **Back** to return to the **Patient** list.

Summary results



The test summary gives an overview of the test result. The diagrams following illustrate the features of test summary screens.

The number of tests currently saved to the patient is displayed in the top right of the screen.


The up and down arrow indicators to the left of the screen show that there are other saved test records for this patient. The left and right arrow indicators display the details for this patient.

Select **Print** to print an individual test record.


Choose **Select** on a test summary screen to analyse the test result in detail.

Select **Back** at any time to exit the test summary screen and return to the **Patient** list to review tests of an alternative patient.


DPOAE test summary screen

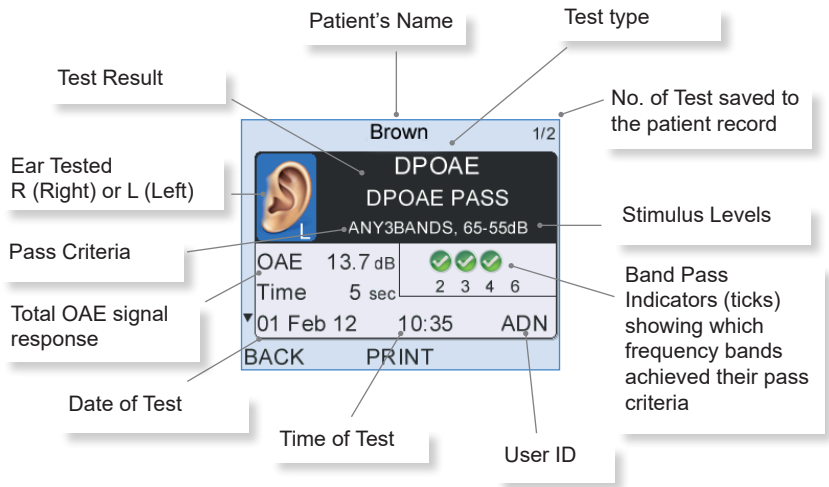

TEOAE test summary screen

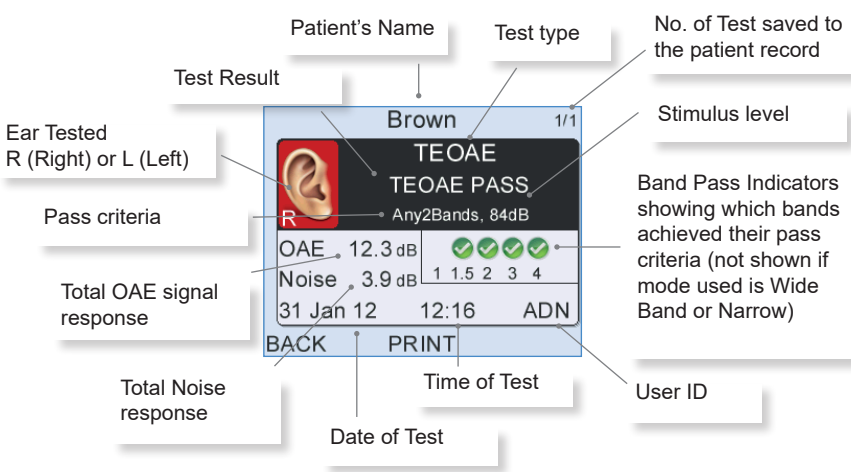

ABR test summary screen

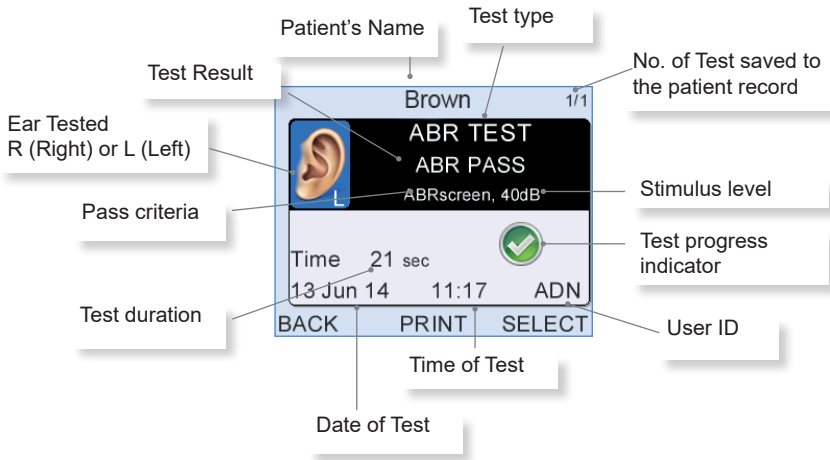

Detailed results

14.4





Test results can be reviewed in detail by choosing **Select** on the test summary screen. The OAE test data is shown on three test screens.

Use the left and right arrow keys to scroll between the screen choices.

Select **Back** at any time to exit and return to the test summary .

Select **Print** to print results (see chapter 16 **Printing**).

15 Configuration

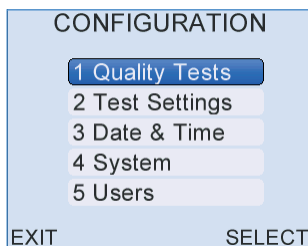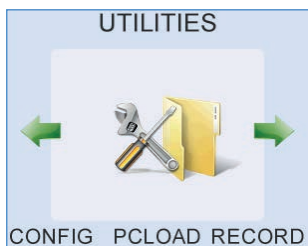

The **Configuration** menu is available from the **Utilities** screen.

Select **Quality Tests** to check the performance of the probe or the ABR electrode cables.

Select **Test Settings** to change test display and pass criteria.

Select **Date & Time** to set the current date and time.

Select **System** for memory, battery and system information.

Select **Users** for login options.

Note:

Users without Admin rights will only have access to **Quality Tests**. The other items will be hidden.

Quality tests

15.1

Details of how to perform the probe and electrode cable tests are in chapter 17 **Quality tests**.

15.2 Test settings

15.2.1 Mode select

MODE SELECT		
Screen	◀	Off ▶
Clinical	◀	On ▶
CANCEL EDIT SAVE		

The test settings are divided into **Screen** and **Clinical** modes. The default settings for each are listed at the end of this section (15.2.10 **Test Mode Defaults**).

Either **Clinical** or **Screen** modes may be turned off. If they are turned off then these modes will not be available for test. To turn a mode off use the up or down arrow keys to select **Screen** or **Clinical** then the left or right keys to display **Off**.

Select **Edit** to change the settings for either mode.

Select **Save** to keep your changes or **Cancel** to discard them.

15.2.2 Clinical and Screen settings

CLINICAL SETTINGS

1 General

2 TEOAE

3 DPOAE

4 ABR

BACK
SELECT

SCREEN SETTINGS

1 General

2 TEOAE

3 DPOAE

4 ABR

BACK
SELECT

The test settings area for each mode is divided into **General** settings, which affect all tests, and settings that affect only OAE or ABR tests. Stop criteria are dependent on both the general and mode specific settings.

Clinical and **Screen** modes have identical set up options but the defaults for each are optimised for different uses.

15.2.3

General


Use the arrow keys to navigate and choose between the setup options (described below).

Select **Save** to apply the settings changes you have made and return to the **Configuration** screen.


Select **Cancel** to discard changes made to settings and return to the **Configuration** screen.

Display

If **dB SPL** is selected a bar chart showing signal and noise at each frequency is displayed during testing.

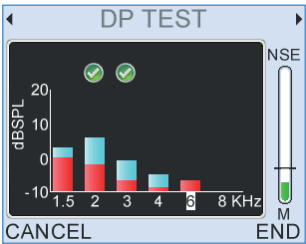


If **Circles** is selected, each circle represents the SNR recorded at a particular frequency.

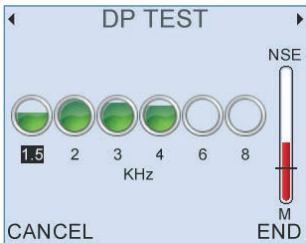

Whichever setting is chosen as default, the other option is available during the test as a side screen, accessed using the left and right arrow keys.

The **Circles** display is not available in **DP 12 Freq** mode.

Neonate mode

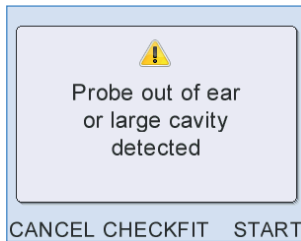

With **Neonate** mode **On** the user is warned if the response from the probe indicates a large ear canal. This provides an additional check of probe fit for users who are testing only babies.

The warning message is displayed after Checkfit and before the test starts. Selecting **Start** will start the test as normal. **Checkfit** returns the user to Checkfit. **Cancel** returns the user to the main test screen.



Ear canal cavities greater than around 0.5cc will trigger the warning.

With **Neonate** setting **Off** (default), no warning message is displayed if a large ear volume is detected.

NReject

The threshold above which data is rejected can be fixed at **High**, **Medium** or **Low**. Alternatively, **Variable** can be selected allowing the reject level to be adjusted during Checkfit and test.

Extend

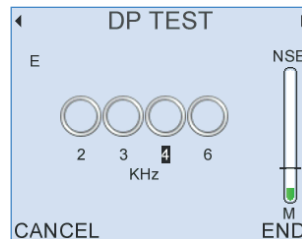

If **Extend** is **On**, the user has the option to extend the test beyond the normal maximum duration. This may be useful if the test result is very close to meeting the pass criteria at the normal test end. If **Extend** is **On**, the central key on the Otoport will show **Extend** when there is around 15

seconds of test time remaining. If the central key is pressed, an **E** will be displayed and the test will run until autostop criteria are met, it is manually stopped or the absolute limit for testing is reached.

Noise mode

Noise mode sets the method by which the noise floor in DP tests is calculated.

The **Standard** mode implements a noise floor which is appropriate for **clinical** measurements in which high accuracy (in terms of the dB SPL of the OAE) is required at each frequency. A good Signal to Noise Ratio (SNR) in this mode indicates that a high accuracy of measurement has been reached.

The **Rapid** mode is appropriate for secure detection of the presence of OAEs at a set number of frequencies for **screening** purposes. A good Signal to Noise Ratio (SNR) in this mode indicates high confidence level that an OAE is present.

The Standard mode can also be used for screening but only in quiet test conditions. Tests will take longer than the Rapid mode and the confidence level of the result will exceed that needed for screening.

Otodynamics does not recommend the Rapid mode for clinical measurements as the dB SPL accuracy may not be sufficient to quantify changes over time.


Further details of the Noise Modes are included in chapter 26, **Mode of operation**.

ABR mains


ABR mains sets the ABR test configuration for optimum test recording in mains (powerline) noise. The mains frequency varies in different countries. Set **50Hz** if the mains in your region is 50Hz and **60Hz** if your region is 60Hz. Set **Not Set** if you are unsure of the mains frequency in your region.

Setting ABR mains from the main menu

If ABR mains is Not Set then you will be prompted to set it when an ABR test is selected from the main menu:

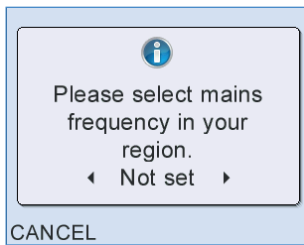

Use the arrow keys to choose 50Hz or 60Hz then press Select. You will be prompted to confirm whether to 'Always use this setting?':

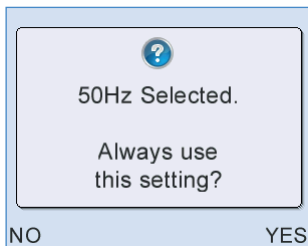

Select **No** if you are unsure of this setting and wish to leave ABR mains Not Set. Select **Yes** to permanently change the ABR Mains setting.

15.2.4

Selecting the appropriate stimulus level

Otodynamics instruments differ in the facility to change stimulus levels.

Where the stimulus is pre-set and unchangeable on a screening instrument, the stimulus level will have been chosen on the basis of independent trials reported in the literature which reliably alerts to the possibility of a mild loss.

Where the stimulus level is changeable on an instrument it is important to select the stimulus level appropriate for your purposes. For screening, the level selected will affect the sensitivity of the device to mild losses. A stronger screening stimulus will result in some patients with mild cochlear losses passing a screening test. For clinical diagnostic purposes stronger stimulation can be useful in identifying residual outer hair cell function with mild to moderate losses.

15.2.5

Selecting levels for TEOAE screening

- For TEOAEs a peak equivalent stimulus level of 84dB SPL has been extensively tested in controlled screening trials and found to detect mild losses. This level is currently adopted by major infant screening programs, as the initial screen, followed up by AABR screening at either 35 or 40dB HL.

TEOAE

TEOAE test is an optional feature in some regions

The **TE Quick** setting is used to switch the TE mode **on** (default) and **off**. When **on**, the mode will provide a Quickscreen click stimulus of **84dB**. If it is set to **off**, this test mode will not be available.

Mode

Mode sets the pass criteria for screening.

The **Wide Band** setting requires a signal to noise ratio (SNR) of 6dB over the 841-4757Hz frequency range in order to meet the pass criteria.

The **Narrow** setting also requires a signal to noise ratio (SNR) of 6dB over the 841-4757Hz frequency range in order to meet the pass criteria. However this setting uses a filter of 1.6-3.2kHz and a stimulus response window 4-10ms to reduce the impact of environmental noise on the recording. This makes this setting particularly appropriate for screening in noisy environment.

The **Any 2 Bands**, **Any 3 Bands** and **Any 4 Bands** settings require a 6dB SNR and a minimum signal level of -5dBSPL in each of the stated number of half octave frequency bands to meet the pass criteria.

In order to meet the pass criteria, all test modes require a minimum total (wide band) signal level of 0dBSPL and the amount of data collected to reach the minimum number of sweeps.

The fixed and configurable test parameters are summarised in the following tables:

Configurable test parameters

Name	Any 2	Any 3	Any 4	Wide	Narrow
Min pass bands	2	3	4	None	None
Min total (wide band) SNR	None	None	None	6dB	6dB
Min SNR per pass band	6dB	6dB	6dB	None	None
Filter (Hz)	1189-4757	1189-4757	1189-4757	1189-4757	1600-3200
Response Window (ms)	2-5-12.5	2-5-12.5	2-5-12.5	2-5-12.5	4-10

The default setting is **Any 2 Bands**. However, it is recommended that you carefully choose pass criteria which suit your program requirements.

Fixed test parameters

Min sweeps (NLo)	30
Min total (wide band) OAE signal	0dBSPL
Min band signal	-5dBSPL
Stimulus level	84 +/- 1dB pe
Max test time	300 seconds
Max low noise (NLo) sweeps averaged	260 sweeps of 16 stimulus presentations
Ring reject	-20dB

Max ratio of stimulus peak to the level 3ms after stimulus presentation.
Stimulus ring can hamper accurate OAE measurement

Input filter	1600-3200Hz - narrow mode only or 1189Hz - 4757Hz
--------------	--

The attenuation at these frequencies is 3dB. Attenuation increases by 80dB/decade below and 40dB/decade above these frequencies

Norms

TE **Norms** are set and displayed in the same way that DP Norms are set.

Start

With start mode set to **On** (default), the testing will proceed from **Checkfit** to **Test** as soon as the Otoport detects a stable probe fit, without the need for the user to select **Start**.

With the **Start** setting **Off**, the user must initiate the test by selecting **Start** when the probe fit and test conditions are satisfactory.

Irrespective of the **Start** setting, the **Start** button is available in order that the user can initiate a test.

Stop

The **Stop** setting controls whether the test automatically stops when the pass criteria are met. If **Stop** is turned **Off**, the test will run for longer, but the OAE levels will be more accurately measured. If **Stop** is **On** when screening, the test will be as short as possible.

15.2.7


Selecting levels for DPOAE screening

- For DPOAEs L1, L2 levels of 65/55dB SPL is most commonly used for hearing screening. Many studies have confirmed the appropriateness of these levels.
- Gorga et al found that L1/L2 stimulus levels of 65/55dB SPL "resulted in the greatest separation between normal and impaired ears. (See "The use of cumulative distributions to determine critical values and levels of confidence for clinical distortion product otoacoustic emission measurements" Michael P. Gorga, Lisa Stover, and Stephen T. Neely, in The Journal of the Acoustical Society of America 100, 968 (1996).
- The appropriateness of stimulus levels 65/55 was confirmed by Stever et al who also noted that levels of stimulus f2 (L2) between 50 and 60dB SPL were "optimum for separating normal hearing from hearing impaired ears" provided that L1 was made 10dB higher than L2. That corresponds to settings of 60/50, 65/55 and 70/60dB SPL. (See "Toward optimizing the clinical utility of distortion product otoacoustic emission measurements", The Journal of the Acoustical Society of America 100, 956 (1996); Lisa Stover, Michael P. Gorga, and Stephen T. Neely.
- Stimulus level adjustments are provided on some instruments so that locally preferred levels can be used.

DPOAE stimulus levels of 70dB SPL and above (e.g. 70/70dB SPL) should NOT be used for screening as it will be insensitive to mild losses. These higher levels ARE useful for clinical investigations, demonstration and training.




15.2.8

DPOAE

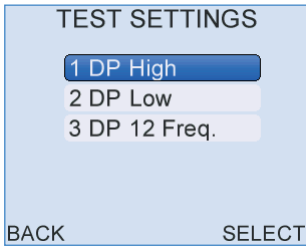

The Otoport Flexi has three different DPOAE test modes, **DP High**, **DP Low** and **DP 12 Freq.** Choose the mode you wish to edit from the menu.

DP Levels

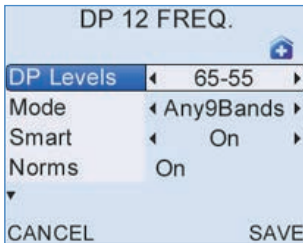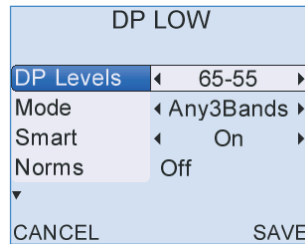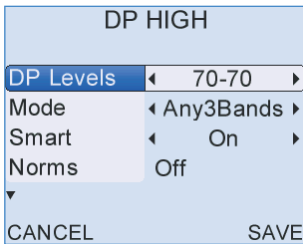

Configuring **Levels** sets two DP stimulus pairs (L1 and L2), which are available for selection prior to test. Stimuli in **DP High** must be of a higher intensity than those set in **DP Low**.

Note:

It is not possible to set the **DP High** mode stimulus settings lower than the **DP Low** mode stimuli and vice versa, but they may be set to equal levels. Stimulus settings are automatically corrected if they do not obey this condition.

If either mode is set to **Off** then this mode will not be available for selection from the main menu.

Mode

Mode sets the pass criteria for screening.

The **Any 2 Bands**, **Any 3 Bands**, **Any 4 Bands** and **Any 5 Bands** settings require a 6dB SNR and a minimum signal level of -5dBSPL in each of the stated number of half octave frequency bands to meet the pass criteria.

If you have selected the frequency range 2-6K, which has four test points, do not choose a pass criteria of **Any 5 Bands** as it will not be possible for the test to meet the pass criteria.

DP 12 Freq mode can be set at **Any 2** to **Any 12 Bands**.

Fixed test parameters

Min band signal	-5dBSPL
Max test time	Approx 90s
Min DP loops (Min no. of completed frequency cycles)	2

The default setting is **Any 3 Bands** for DP High and DP Low and **Any 9 Bands** for DP 12 Freq. However, it is recommended that pass criteria are carefully chosen to suit the particular OAE testing programme.

Smart

With **Smart** mode **On**, DP bands that have met the pass criteria or bands that have reached a low noise level (-12dB) will be skipped in the frequency presentation loop, improving test efficiency by allowing more time for the remaining frequencies.

Norms

Norms allows the user to set the expected range of OAE response levels. This range is then marked on the DP-gram or bar-chart screen during tests as a visual aid.

Setting **Norms** does not affect any pass criteria that has been set. Pass criteria are based on signal-to-noise ratios and are intended for screening applications or for data quality control. Norms are based on dB SPL values and are intended to aid clinical interpretation.

Normative OAE levels are dependent on the test population (particularly their age) and on test settings (particularly stimulus levels). Norms may be set in any test mode but default values are only set for the DP 12 Frequency test. The default values provided were derived by interpolation from data listed here:

<http://www.hearingreview.com/2013/10/an-overview-of-oaes-and-normative-data-for-dpoaes/>

The default norm levels in the Otoport represent the range from the 10th to the 90th percentile of the test population (aged 18-25). This means that 80% of DPOAE levels should be between these marked norm levels. These norms values are provided for indication only; you should develop your own norms locally by collecting results from individuals within your target population with normal hearing, or by consulting the literature.

When **Norms** is highlighted, press the right arrow key to edit the values. A pop-up table appears showing **Low** (minimum) and **High** (maximum) Norm levels for each test frequency. All Norms default to **Off**. Use the left and right arrow keys to set the Norm level (range -10 to 20dB SPL). Use the up and down arrow keys to change between frequency. Selecting **Down** at the bottom of the **Low** column provides access to the **High** column. Selecting **Up** at the top of the **High** column allows access to the **Low** column settings.

Select **Back** when you have finished editing the **Norms**.

Freq range

The frequency range tested may be selected with the left and right arrow keys.

1.5-8k tests at six F2 frequencies: 1.5, 2, 3, 4, 6 and 8kHz

1-6k tests at six F2 frequencies: 1, 1.5, 2, 3, 4 and 6kHz

2-6k tests at four F2 frequencies: 2, 3, 4 and 6kHz

The frequency range for DP 12 Freq is fixed at 1-8kHz.

Start

With start mode set to **On** (default), the testing will proceed from **Checkfit** to **Test** as soon as the Otoport detects a stable probe fit, without the need for the user to select **Start**.

With the **Start** setting **Off**, the user must initiate the test by selecting **Start** when the probe fit and test conditions are satisfactory.

Irrespective of the **Start** setting, the **Start** button is available in order that the user can initiate a test.

Stop

The **Stop** setting controls whether the test automatically stops when the pass criteria are met. If **Stop** is turned **Off**, the test will run for longer, but the OAE levels will be more accurately measured. If **Stop** is **On** when screening, the test will be as short as possible.

Band SNR

Band SNR sets the minimum Signal to Noise Ratio required in each band before that band passes. The SNR calculated is dependent on the noise mode used (see 15.2.1 **Noise mode**). By default, it is set to 6dB SNR.

15.2.9

ABR

TEST SETTINGS

1 ABRscreen

2 ABRcustom

BACK

SELECT

ABRscreen

Stim Level 40 dBHL

Pass Criteria ◀ PC2 ▶

Ear Cups ◀ Auto ▶

ABR Mains ◀ 50Hz ▶

CANCEL

SAVE

ABRcustom

Stim Level 30 dBHL

Pass Criteria ◀ PC1 ▶

Ear Cups ◀ Auto ▶

ABR Mains ◀ 50Hz ▶

▼

CANCEL

SAVE

ABRcustom

▲ Stim Type ◀ Click ▶

Start ◀ Off ▶

Stop ◀ Off ▶

Neonate ◀ Off ▶

CANCEL

SAVE

The Otoport OAE+ABR has two different ABR test modes, **ABRscreen** and **ABRcustom**. ABRscreen is optimised for the screening of neonates and is less configurable than ABRcustom. Choose the mode you wish to edit from the menu.

Stim level

‘Stim Level’ sets the stimulus level used in the ABR test in dBHL.

If Stim Level is set to OFF then the selected mode (ABRscreen or ABRcustom) is not available for testing and it will not appear in the main menu carousel.

The ABR Screen mode is intended for newborn hearing screening.

The default setting is 40dBHL. You should set this level only if directed to you by your screening program manager.

The stimulus level should be set to the lowest value compatible with the aims and targets of the hearing screening program. For high sensitivity detection of even slight hearing impairments the Otoport 35dBnHL setting has been successfully used. At this stimulus level the number of unnecessary referrals (i.e., false positives) will be higher than with 40dBHL stimulation. Many major infant screening programs (e.g., UK English, and Welsh national programs) use the 40dBHL setting. They find it gives both good sensitivity to mild and clinically significant losses with an easily manageable refer rate. Typically, in the well-baby population, an OAE test fail is immediately followed up by an AABR screen using the Otoport. Note that screening with stimulus levels significantly above 40dBnHL is likely to miss some mild hearing losses.

In ‘**ABRcustom**’ mode the stimulus level can be set from 5-60dBHL in 1dB steps. The default setting is OFF (i.e. ABR custom mode test is unavailable).

- The ABRcustom mode is not intended for diagnostic use or ABR threshold determination.
- Stimulus levels higher than 45dBnHL can be useful in training sessions and in instrument function confirmation testing to allow more rapid acquisition of ABR in noisy environments. These levels should not be used for infant screening as they will miss mild to moderate losses.
- Fine adjustments of the stimulus level (1dB steps) are intended for the setting of precise (custom) stimulus levels e.g. for compatibility with prior screening practice.
- Low stimulus levels (down to 5dBnHL) can be used for the audiological

confirmation (subjective testing) of the instrument's hearing level setting calibration.

In **Ear Cups** mode the stimulus level limits are 40 dBHL when the stimulus type is chirp and 30 dBHL when the stimulus type is click.

Notes:

The Otoport OAE+ABR dynamically adjusts the delivered sound pressure level to achieve the selected normal hearing level (nHL) for each test. The instrument will achieve the selected dBnHL in all sizes of ear including, for screening levels (30-45dBnHL), adult ears up to the volume of a neonate screening ear cup.

The Otoport OAE+ABR is capable of recording ABR responses from patients of all ages provided a non-template (Fsp only) pass criteria is selected (PC1 or PC4). However the specificity of the device has only been established for neonates and therefore it is not intended for use as screen for hearing loss in older children or adults.

Stim Type

Stim type sets the stimulus type used in the ABR test. The types available are 'click' and 'chirp'. See chapter 26 **Mode of operation** for further details of these stimulus types. The chirp stimulus has been demonstrated to give a larger ABR response for the same stimulus level. Stim Type is configurable only in ABRcustom, default is chirp in both modes.

Start

If **Start** is ON then the ABR test will proceed from the Impedance Check screen to data collection (autostart) without any action from the tester if test conditions are good.

If Start is OFF the tester determines when to proceed from Impedance Check to data collection (manual start).

Start is configurable only in ABRcustom, default is ON in both modes.

Stop

The **Stop** setting controls whether the test automatically stops when the pass criteria are met. If **Stop** is turned OFF, the test will run for longer,

but the ABR levels will be more accurately measured. If **Stop** is ON when screening, the test will be as short as possible.

Stop is configurable only in ABRcustom, default is ON in both modes.

Pass criteria

Pass criteria sets the conditions in which the ABR test will give a pass result.

Pass criteria is based on a statistical measure similar to signal to noise ratio known as Fsp, and a measure of the extent to which the averaged response waveform resembles a typical neonate ABR, a value referred to as template correlation (TC).

Fsp is the principle determinant of a Pass. It must achieve a minimum *fixed Fsp* or *dynamic Fsp* level. The *dynamic Fsp* threshold rises if power line noise is a large part of the electrical noise measured in order to account for any possible contribution of the powerline noise to Fsp (to ensure that the powerline noise is not mistaken for an ABR). The minimum *fixed Fsp* threshold is higher than the largest Fsp ever likely to be achieved by chance in EEG noise.

The *minimum TC* requirement should be achieved when recording an ABR waveform from a neonate (34 weeks to 6 months gestational age). The *strict TC* requirement is higher than largest TC ever likely to be achieved by power line interference.

The two measures Fsp and TC are combined in four different ways as follows:

PC1 requires:

Fsp level exceeds the dynamic Fsp with no template requirement

PC2 requires:

Fsp level exceeds the dynamic Fsp and TC exceeds the minimum TC level

PC3 requires:

Fsp level exceeds the dynamic Fsp and TC exceeds the minimum TC level

Or

Fsp level exceeds the minimum Fsp and TC exceeds the strict TC level

PC4 requires:

Fsp level exceeds the dynamic Fsp with no template requirement

Or

Fsp level exceeds the minimum Fsp and TC exceeds the strict TC level

When to use each PC

PC1 is ideal for performing an ABR test on adult subjects and is the default setting for ABRcustom mode. It is useful for training, demonstration and clinical investigations.

PC2 is designed for neonate screening and is the default setting for the ABRscreen mode.

PC3 and PC4 may give higher specificity in challenging noise environments, potentially passing healthy ears securely even when interference levels are high. Both are designed for neonate screening but PC4 can also be used with adult ears.

Ear Cups

This setting allows the use of ear cups and it can be set in three different ways :

OFF – Will always go into test assuming ear cups are not being used.

AUTO – Will detect whether ear cups are being used and prompt the user before test if ear cups are being used or not.

ON – Will always go into test assuming ear cups are being used.

15.2.10

Test mode defaults



Screen Mode Clinical Mode

General	Display	Circles	Bars
	Neonate	On	Off
	Nreject	Variable	Variable
	Extend	Off	On
	Noise Mode	Rapid	Standard
TEOAE	TE Quick	84 dBpe	84 dBpe
	Mode	Narrow	Any2Bands
	Norms	Off	Off
	Start	On	On
	Stop	On	Off
DP High	DP Levels	Off	70-70
	Mode	Any3Bands	Any3Bands
	Smart	On	On
	Norms	Off	Off
	Freq range	1.5-8k	1.5-8k
	Start	On	On
	Stop	On	Off
DP Low	Band SNR	6	6
	DP Levels	65-55	65-55
	Mode	Any3Bands	Any3Bands
	Smart	On	On
	Norms	Off	Off
	Freq range	1.5-8k	1.5-8k
	Start	On	On
	Stop	On	Off
	Band SNR	6	6



Screen Mode

Clinical Mode

DP 12 Freq	DP Levels	Off	65-55
	Mode	Any9Bands	Any9Bands
	Smart	On	On
	Norms	Off	On
	Start	On	On
	Stop	On	Off
	Band SNR	6	6
ABR Screen	Stim Level	40 dBHL	Off
	Pass Criteria	PC2	
	Ear Cups	Auto	
ABR Custom	Stim Level	Off	Off
	Pass Criteria	PC1	PC1
	Ear Cups	Auto	Auto
	Stim Type	Chirp	Chirp
	Start	On	On
	Stop	On	On

15.3

Date and time

DATE & TIME		
Time	10:46	24Hr
Date	01 Feb 2012	
Format	◀dd.Mmm.yyyy▶	
<div>CANCEL</div> <div>SAVE</div>		

The date and time set on the device can be altered in the **Date & Time** screen. Use the keypad to change the **Time**.

When the **Date** field is highlighted press the right arrow key to access the calendar pop-up table. The day will be highlighted first and can be altered using the up and down arrow keys. Continue to use the left and right arrow keys to jump between the Day/Month/Year and the up and down arrow keys to select the required date.

The date **Format** can be changed between dd.Mmm.yyyy and mm.dd.yyyy or dd.mm.yyyy via the choice bar.

Select **Save** to set the current date and time settings and return to the **Configuration** screen.

Select **Cancel** to discard changes made to date and time settings and return to the **Configuration** screen.

Important Note:

Do not set the date on the Otoport to an earlier date, if there is data stored on the device.

15.4


System



The **System** screen allows users to view information on **Memory Status**, **Controls**, **Battery** power, **System Information** or to change the **Setup**.

15.4.1

Memory status

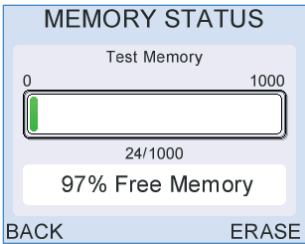

The Otoport has the capacity to store up to 1,000 test records. The memory status screen displays the number of records currently stored and the percentage of memory still available.

Selecting **Erase** deletes all test records from the Otoport after requesting confirmation from the user. A screen confirming the **Erase** is then displayed and the user is returned to the main menu.

If there is less than 10% free memory then the **Memory Status** screen will be displayed at start up.

When 0% free memory is reached, the **Memory Status** screen will be displayed and no further tests may be performed until tests have been erased.

The **Memory Status** screen will be displayed immediately after the 900th result has been saved warning the user that there is limited storage capacity left.



If the **Memory Status** screen has been displayed because the Otoport memory is full or nearly full, the user will be prompted to **Download** data to a PC using Otolink (see the separate **Otolink User Manual**).

15.4.2

Controls



Volume

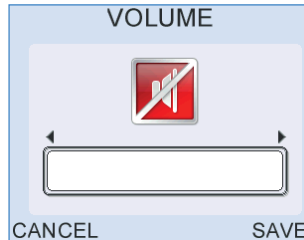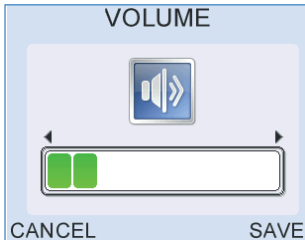

The current **Volume** level is represented on the display by a number of shaded blocks. Use the **Left/Right Arrow** buttons to decrease or increase the **Volume** level. To turn the sound off press the left arrow key repeatedly until **Sound Off** appears in the centre of the display.

Select **Save** to accept the new **Volume** level.

Select **Cancel** to ignore changes and return to the **Controls Menu**.

Brightness




The screen **Brightness** can be altered by pressing the left/right arrow keys.

Select **Save** to accept the adjusted **Brightness** level.

Select **Cancel** to ignore changes and return to the **Controls Menu**.

Backlight

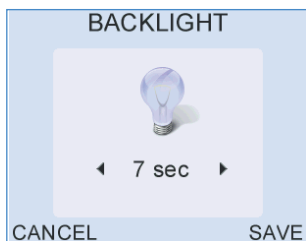


Use the left and right arrow keys to toggle between the **Backlight** control choices for the screen and keypad. The backlight can be configured to be either always **on** or **off**, or **on** for a specific period of time (7, 10, 20 or 30 seconds) after a button press. Reduction in the backlight time will help to preserve battery charge during operation.

Select **Save** to accept the **Backlight** setting.

Select **Cancel** to ignore changes and return to the **Controls Menu**.

15.4.3

Battery

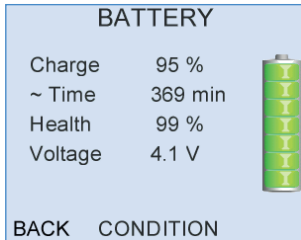

The **Battery** screen provides information on the current battery status. The total battery power remaining is displayed as a percentage and as an approximate operation time. The calculated time is only an approximate indication as the power requirements will vary depending on the mode of operation.

The battery graphic on the right of the screen conveys the total remaining power. The battery segments are shaded according to the following criteria:


Segments Displayed	Battery Power (%)
7	95 - 100
6	75 - 94
5	55 - 74
4	40 - 54
3	30 - 39
2	20 - 29
1	10 - 19
0	< 10

The battery **Voltage** and **Health** are provided as a diagnostic tools.

The battery graphic is also displayed on the **Logo** screen to inform the user of the battery power every time the device is switched on.

Select **Condition** to discharge the Otoport battery. See chapter 21 **Otoport power** for more information.

Setup

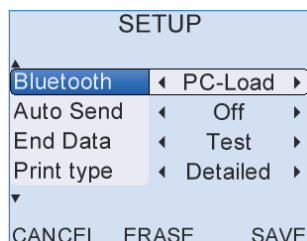

Quick Save

The options available from the test result screen depend on the **Quick Save** option.

If **Quick Save** is **On**, test results can be saved from the test result screen with a single button push but patient details can only be entered after testing by selecting **Last** on the main menu.

If **Quick Save** is **Off**, options to enter patient details before testing and to review the test result before the test is saved are available (see section 11.1 **Quick save option**).

Bluetooth



Bluetooth sets how the Otoport's wireless communication will be used.

If **Bluetooth** is set to **PC-Load** then the Otoport can use Bluetooth communication to send test results to a PC. Details of how to set up wireless download to PC are included in your Otolink manual.

If **Bluetooth** is set to **Print** then the Otoport can use Bluetooth communication to send test results to the mini-printer (see chapter 11 **Printing**).

Wireless printing and download are only available on Bluetooth enabled Otoports. You can tell if a Bluetooth module is fitted, as a Bluetooth symbol (shown above) is included on the product label on the back of the Otoport. If **Bluetooth** is set to **None** then the Otoport cannot take advantage of the Bluetooth Communication for either Print or PC-Load as it does not contain the necessary hardware.

The function of the **Auto Send** and **End Data** options below are dependent on this setting.

Auto Send

If **Auto Send** is set to **On** then the test result is automatically printed/downloaded after the test is saved.

If **Auto Send** is set to **Off** then the user has the option to print/download the test after save.

End Data

If **End Data** is set to **Patient**, then all the test results for the current patient are printed at the end of the test.

If **End Data** is set to **Test**, then only the last test performed is printed at the end of the test.

Select **Save** to accept the setting and **Cancel** to discard any change.

Note:

To avoid printout duplication, it is not possible to set **Auto Send** to **On** and **End Data** to **Patient**.

Print

If **Print** is set to **Automatic**, the test result is automatically printed after the test is saved.

If **Print** is set to **Manual**, the user has the option to print the test after saving.

End Print

If **End Print** is set to **Patient**, all the test results for the current patient are printed at the end of the test.

If **End Print** is set to **Test**, only the last test performed is printed at the end of the test.

Note:

To avoid printout duplication, it is not possible to set **Print** to **Automatic** and **End Print** to **Patient**.

Print type

Print type controls the length and detail contained in the Otoport printout. The **Summary** format prints only core patient and test details. The **Detailed** format prints a fuller set of patient and test quality details (see section 16.2.3).

On connect

On connect printing allows printing to be initiated as soon as a wired printer is connected. This is particularly useful if the Otoport is used with a Docking Station as it allows results to be printed as soon as the Otoport is dropped into the docking station.

On connect may be turned **Off** or set to print the last **Test**, all unprinted tests for the last **Patient**, or **All** unprinted tests.

Printing will only start if the Otoport is on and displaying one of the main module screens.

If **Cancel** is selected during the print, three options are available:

If **Cancel Print** is selected, the Otoport will not attempt to automatically print the test(s) again (test may still be selected to be printed manually).

If **Retry** is selected then printing will recommence.

If **Stop On Connect** is selected then the **On connect** setting is turned off and the Otoport will not attempt to print tests on connection in future.

Worklist

The **Worklist** allows details for multiple patients to be entered into the Otoport prior to testing. If **Worklist** is set to **On**, the list is accessible from the main menu (see chapter 13). If the **Worklist** is set to **Off**, it is not available.

Language

Select the language you require using the left and right arrowkeys.

15.4.5

System info

The **System Info** area provides information on the Otoport.

System Details displays information for Otodynamics engineers (see chapter 22.3 **System details** for further details).

The **About** screen provides information relating to the Otoport's identification and mode of operation including the model variant name.

The firmware revision number and issue date are stated, together with the unit's unique **Hardware ID** and machine ID (**GSN**). The next scheduled Calibration Due date is also shown. A dash is shown if no calibration date has been set.

ABOUT	
Otoport Advance	
Revision	1.16.1.30A
Issued	Oct 2 2014 10:44:37
Hardware	0000105367B5
GSN	TPW
Calibrate by	03 Nov 2014
BACK	

Select **Back** to return to the **System** menu.

15.5

Users

USERS	
1 Add New User	
2 View Users	
3 Settings	
BACK	SELECT

Select **Add New User** to enter details of a new user and save to the user list. Adding users to the Otoport allows test results to be attributed to individuals and allows password control of areas such as Test Setup.

Select **View Users** to review, edit or delete users from the current **User List**.

Select **Settings** to turn **Login** on or off.

Select **Back** to return to the **Configuration** menu screen.

15.5.1

Add New User

To add a **New User**, complete the field entries shown on the **New User** screen. The following table describes the field choices available:

Field	Description	No. Characters
Name	User's name that appears at Login	1-8
User ID	The user's unique identification This is attached to a test record when saved to the database	3 (capitalised only)
Password	An alphanumeric password required for secure login (optional)	0-8 (capitalised only)

The **User ID** is added to a saved test record to identify the user who performed the test. The **User ID** must therefore be unique and the message **Cannot Save! User ID already exists** will appear on **Save** if the chosen **User ID** is already associated with a current user. The device will return to the **New User** screen where the **User ID** field will be selected for editing.

Selecting **Save** will add the user to the user list. The user list will appear with the newly saved user highlighted on screen. The message **Cannot Save! Please enter Name, and User ID** may appear on press of **Save** if any of these mandatory fields have been left unfilled.

Select **Cancel** to cancel the addition of a **New User** and return to the **Users** menu screen.

A new user is given a choice of two levels of access rights. If **Yes** is selected in the administrator field, then the user will have full access to all the **Config** areas of the device. Select **No** to restrict the user's rights to only the **Probe** test area in **Config**, disabling access to higher level functions.

15.5.2

View user list

The user list displays the **Name**, **Password** and **Status** of all users currently saved to the device.

Select **Back** to exit the user list and return to the **Users** menu.

If a user has been assigned Administrator rights, an **A** will be present in the right hand **Status** column of the table.

15.5.3

Edit user

Select **Edit** to alter the details of a highlighted user.

Select **Save** to save changes to the user's details and return to the user list.

Select **Delete** to remove the selected user from the user list. A confirmation message will appear at the top of the screen. Select **Yes** to confirm the deletion or **No** to retain the user and return to the **Edit User** screen. It is not possible to delete the default "Admin" user.

The message **Cannot Delete! User has tests in database** will appear if there are any patients in the database. It is necessary to delete all patient records from the device prior to deletion of users. Note: Patient results should be downloaded to PC first.

Select **Cancel** at any time to discard changes and return to the user list.

16 Printing and downloading



Test results can be printed on the optional Otoport mini-printer or downloaded to PC for printing, archive or export. Wireless (via Bluetooth) and wired (via supplied cables) connections are available for both functions.

16.1

Bluetooth wireless technology enabled printing and download




Wireless printing and downloading are only available on Bluetooth enabled Otocheck ABR and Otoport instruments. If a Bluetooth module is fitted, a Bluetooth symbol (shown above) is included on the product label. Downloading can also be performed with a wired connection, using the cables supplied.

However, the Bluetooth connection supports *either* printing *or* downloading, not both (see 15.4.4 **Setup** to select which function is available). The softkey **Print** or **PC-Load** is shown on screen whenever the function is available.

Bluetooth download requires that Otolink software is installed and that your Otoport is paired with your PC. The password for pairing is 4679. See your Otolink manual for full instructions. Refer to **Custom Settings** in Otolink manual (currently chapter 15).

When the connection to the PC is ready to send data the **PC-Load** text on the Otoport screen is green:

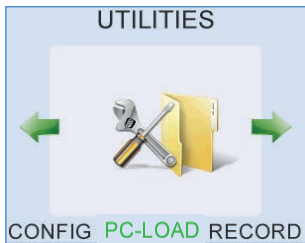

If the connection is not complete then the **PC-Load** text on the Otoport screen is black.

Bluetooth printing is described throughout this chapter.

Bluetooth is disabled when the Otoport is connected to a power supply (non US models only).

16.2

Wired downloading



Wired download is available at any time when a test is not in progress and the Otoport database is not open. See the Otolink manual for details.

16.3

When you can print


The Otoport provides flexible options to print from various areas of the user interface, including printing at the end of the test.

Print settings are located under **Configuration** in **System, Setup**.

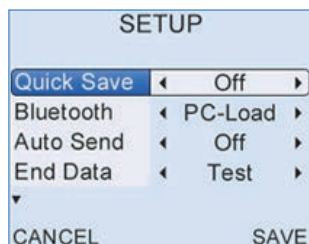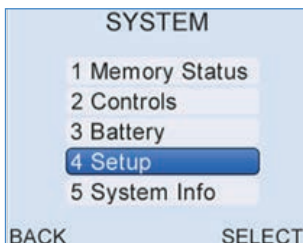

16.3.1

Printing at the end of a test

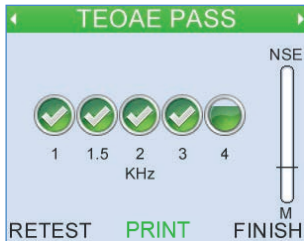



When the OAE recording is finished and the result has been saved, select **Print** for a printout of the patient details and current test result or all the test results for the current patient, depending on the Otoport configuration (see chapter 15).

16.3.2


Printing or downloading from records

Results can be printed or downloaded from the Otoport **Records** area. Select the patient for whom you would like to print/download results (see the **Records** section for details of how to retrieve specific records from the database).


To print or download patient details and all test results for that patient, select **Print** or **PC-Load** on the **Patient Details** screen.

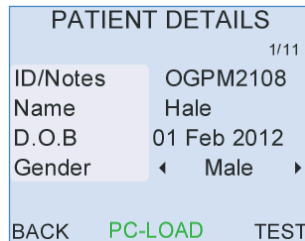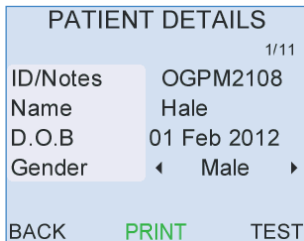

To print or download patient details and the result of a specific test, select the **Results** summary screen, scroll through the different tests for the patient (using the up and down arrow keys) and select **Print** or **PC-Load**.

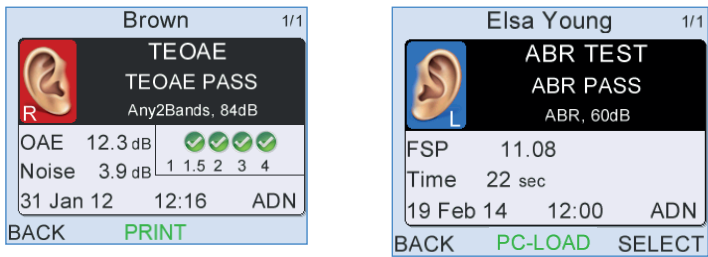


Select **PC-Load** on the **Utilities** menu to download all new records for all patients and tests that haven't previously been downloaded. It is useful to use this option after collecting results over a day's work for instance, when you wish to download all new records for that day.

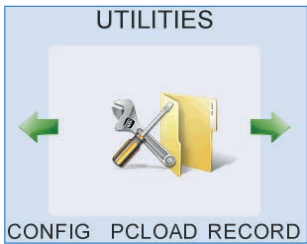


16.3.3

Print type

There are two printing formats provided on the Otoport - **Summary** and **Detailed**. The **Summary** format (below left) prints core patient details and the test results. The **Detailed** format (right) prints all the test details and a fuller set of patient details.

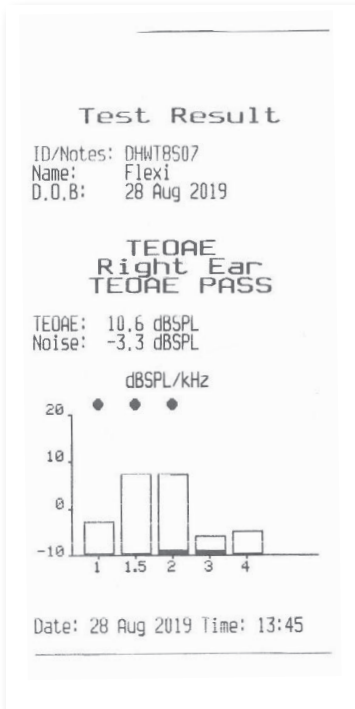

Summary format

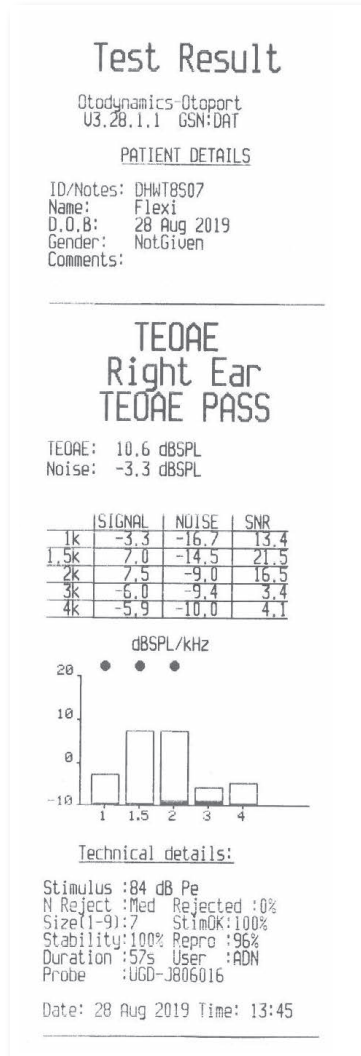


Detailed format

16.4

The printing process

If you are using the wired printing method ensure the printer is connected to the Otoport using the printing cable provided. Connect the flat connector to the Otoport with the arrows facing upwards and the square connector to the back of the printer.

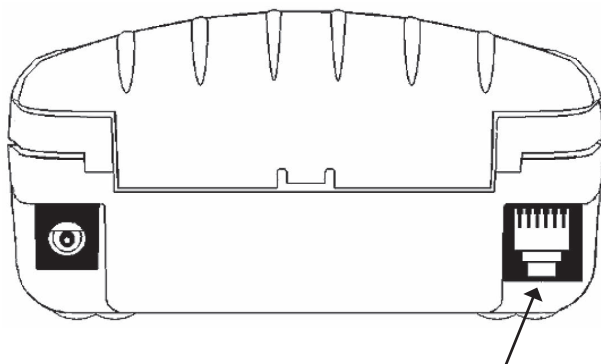

Printer cable socket

The wireless printing method has a range of up to 10m in direct line of sight. It is recommended that the printing distance is reduced to 5m to help ensure robust communication. Remain within this range for the duration of the printout. Printouts will not complete if wireless communication is lost.


The **Print** option will be shown in green if the Otoport is currently connected to a printer wirelessly. Otherwise, the **Print** option is shown in black.

Note:

When using multiple Otoports with wireless connection to a single printer, the last Otoport to print must be switched off before another Otoport can print.

The printer is powered from batteries, or can be connected to mains power when printing. Prior to printing, switch on the printer, using the power button on the top. When the printer is powered, a green light will be displayed. To save power, the printer will automatically switch off after 30 minutes of inactivity. If it is connected to mains power, the printer will remain on indefinitely.


When a print is initiated, the Otoport will establish communication with the printer. The screen **Connecting to Printer** will be displayed.

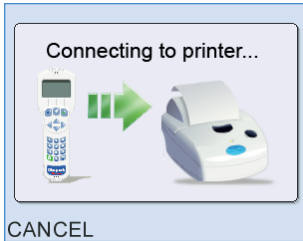

The printout will then commence. When the printout is completed the screen from which the print was initiated will be displayed.

If there is a problem connecting to the printer using the wired method, the message **Printer not connected!** will be shown briefly and then the screen from which the print was initiated will be displayed. Check the printer is connected correctly and switched on then re-try.

If there is a problem connecting to the printer using the wireless method, the following screen will be displayed providing options to cancel, search for an alternative (**Alter.**) or **Retry**.

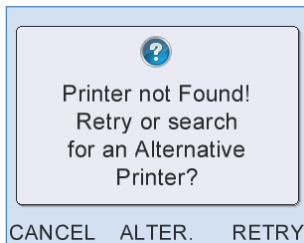

To **Retry** the print, ensure the printer is switched on and is within range (5m). Then select the **Retry** button.

If printing wirelessly and you have an alternative printer available, or if **Retry** is unsuccessful, select **Alter.** The Otoport will search for all available printers, taking up to 30 seconds.

Up to five available printers will now be listed in order of signal strength. The first number displayed on the screen corresponds with the serial number printed on the bottom of the printer. The second number indicates signal strength.

Select the printer required with the navigation keys and then **Select**. Printing will then commence.


To cancel the printout, select the **Cancel** button.

When your print has completed, pull the paper sharply towards you across the serrated tear bar to remove the printout and store it with your patient records.

16.5 Printer fault detection

The printer can detect if the paper roll has run out, or if the lid is open.

The Otoport will report the printer is out of paper and the following message will be displayed.

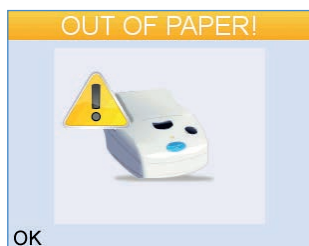

Select **OK** to cancel the print job. Retry the printout when you have rectified the problem.

For wireless printing, print jobs sent to the printer will be stored (spooled) and printed when the detected condition is rectified. The printer's green light will flash when a print job is being stored.

Printer light summary

The light at the front of the printer has a number of colour combinations, which indicate various conditions.

Constant green

Normal operation, running on battery power

Flashing green

The printer is storing print information (spooling) that cannot be printed at the time (e.g no paper, or printer lid open)

Flashing green/orange

Battery is being charged

Red

Low battery or other problem

No light


Unit is in sleep mode, has a flat battery, or the battery is not connected

16.7

Paper

When the printer is switched on, the button provides a paper feed function. A double press of the button will initiate a test print.


The printer is supplied with spare paper rolls. To change the printer roll, pull the lid release catch (1) forwards with your thumb and the paper roll lid will spring open.

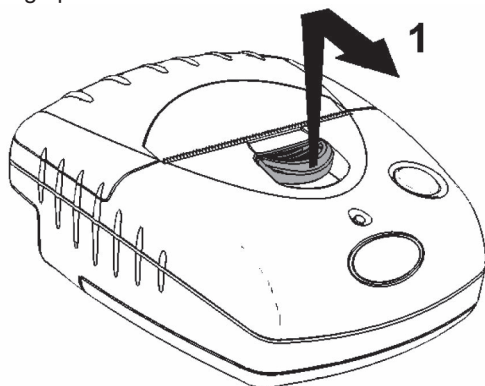

Unwind a small amount of paper from the roll. Insert the new roll (2) ensuring the paper will pass through the paper feed (3) and close the cover with a click.

After loading, check that the paper advances properly using the paper feed function, and tear off any excess by pulling the paper sharply towards you across the serrated tear bar. In the event of a jam or other paper loading problem, release the lid and straighten the paper before closing again.

Self-adhesive paper rolls are also available and may be used in the same way as standard paper, but can be stuck to your patient records.

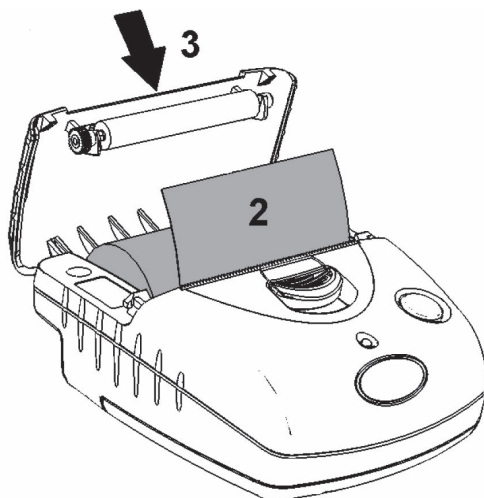


16.8

Charging the printer



To charge the printer, plug the charger into a mains outlet socket and insert the charger jack plug into the rear of the printer. The light on the printer will flash green/orange to show the printer is on charge. The red charger light will also illuminate. A full charge will take approximately 15 hours.

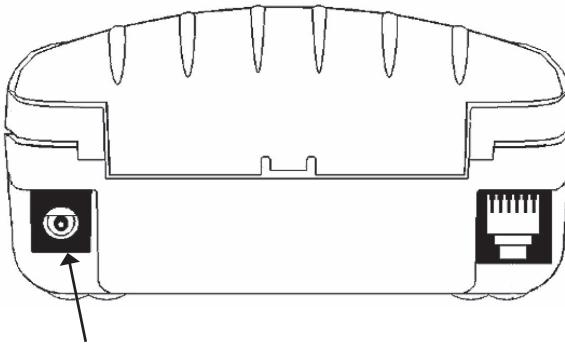

Charger jack plug socket

The printer can be used as normal whilst charging.

Once fully charged, the printer has enough power for around 10 hours standby use. The batteries should provide enough power to print several rolls of paper. The printer light will flash green/red when the batteries are low.

Note:

The printer charger is not medically approved. The Otoport must not be in patient contact if connected to the printer whilst the printer is charging.

16.9



Changing the battery



The printer battery will provide up to 500 charge and discharge cycles. If the battery performance deteriorates the batteries will need to be changed. A spare battery cradle, which takes 4 AAA batteries, is provided with the printer. Alternatively a new battery pack can be obtained from your dealer or Otodynamics.

To change the battery pack:

Remove the screw (1) from the battery compartment cover.

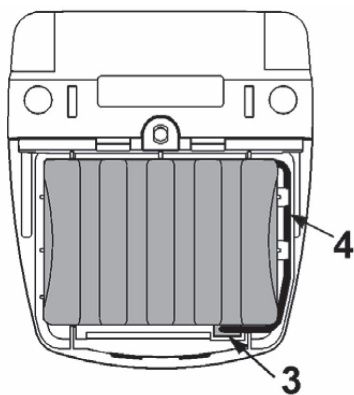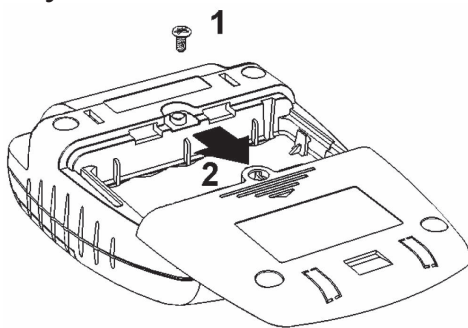

Push down, and slide back the battery compartment cover (2).

Remove the old battery pack and disconnect the battery pack connector, noting its orientation.

Fit the battery pack connector (3) taking care to insert it correctly.

Fit the battery pack ensuring wires (4) are not trapped.

Slide back the battery compartment cover and replace the screw.

Important Note:

Only charge the printer if it contains an approved battery pack, supplied by your dealer or Otodynamics Ltd.

17 Quality tests

Damage or malfunction of the Otoport, the probe or the cables can lead to errors in testing. To ensure that any faults are detected before they lead to faulty data collection, the following tests can be performed.

Quality tests should be carried out on a weekly basis.

There are five different quality tests, described below. The Probe Test and ABR Cable Test are initiated from within the **Configuration** menu; the Cavity, Occlusion and Real Ear tests involve running a standard TEOAE or DPOAE test.

17.1

Probe test



Probe Test is an option accessed from the configuration menu (see chapter 15 **Configuration**).


A **Probe Test** should be performed regularly to monitor the calibration of the probe's output stimulus level and microphone response.

Note:

Probes supplied with a new Otoport system are tested with the system and Probe Test levels are stored. These levels form a baseline to compare future tests against in order to monitor any calibration drift. It is not necessary to save a new baseline level for these probes.

Replacement probes supplied should be tested with your Otoport system and new Probe Test results saved as a baseline reference.

On selection of **Probe Test** the message **Place Probe into Otodynamics Test Cavity. Press OK to begin test.** will appear on screen.

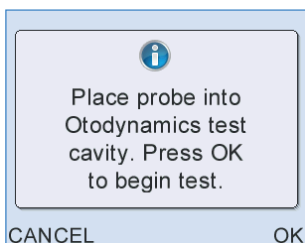

If two probes are connected, then the probe test will run automatically on both, so it is necessary to insert both into test cavities.

Remove the tip from the probe and place the cavity on a flat surface. Insert the probe into the test cavity at a 90 degree angle to the top of the cavity, between the screws, as shown below left. Press the probe firmly into the cavity until the shoulder of the probe touches the top of the cavity. When released, the probe will rise a little to its natural position and the shoulder may no longer touch the cavity. Inserting the probe at the wrong angle or with the probe head over one of the screws may result in incorrect test results.



Select **OK** to begin the **Probe Test** or **Cancel** to return to the **Probe Menu** screen.

The probe outputs sound at 1, 2 and 4kHz for both loudspeakers in the DP probe (**A** and **B**) and the system compares the response at these frequencies against values already stored on the probe.


Checking the probe response against the absolute range determines if the probe is OK for use. Checking the probe response against the probe specific values is more sensitive and provides a warning if the response of the probe has changed.

17.1.1

Results


The possible results of the test are:

Pass

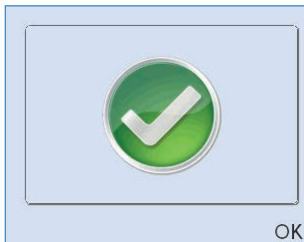

The levels recorded at all frequencies are within the absolute range and within $\pm 3\text{dB}$ of the probe specific values.

Fail

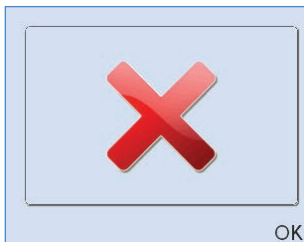

One or more of the levels recorded are outside the absolute range specified for the probe. If a Fail is shown on screen inspect the probe coupler tubes for debris, replace the coupler if necessary and repeat the Probe Test, by selecting **Retest**, ensuring the ear piece is firmly inserted in the test cavity. If the test continues to fail there may be a fault with the probe or system. Contact your dealer or Otodynamics for advice.

Query



The levels recorded at all frequencies are within the absolute range but one or more frequencies is more than ± 3 dB of the probe specific values. If a Query is shown inspect the probe coupler tubes for debris, replace the coupler if necessary and repeat the Probe Test by selecting **Retest**, ensuring the ear piece is firmly inserted in the test cavity. A Query result indicates that there have been changes in the probe but that these changes are not large enough to invalidate testing. It may be possible for the probe calibration to be adjusted if the probe is returned to Otodynamics.

Noisy




There was significant noise during the calibration test. This noise may have influenced the levels recorded so a **Retest** should be performed.


Select **Back** to exit the probe test and return to the Probe Menu screen.

Dual probe result

If two probes are connected to the Otoport, then both are tested and a test result for each is shown:

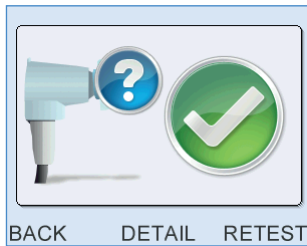

The full test result for either can be selected when **Detail** is selected and a probe icon will show which probe result is displayed.

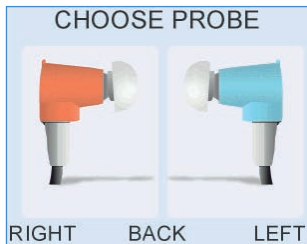

Details

The full test result can be viewed by selecting **Details**. The details screen shows the levels recorded from the probe loud speaker at each frequency tested. The **NEW** column shows the levels just recorded and the **OLD** results are the levels that are stored in the probe.

Results are given for each frequency tested:

PROBE:UGD-C108003					
	A		B		
	OLD	NEW	OLD	NEW	
1 KHz	76.4	75.7	76.5	75.8	✓
2 KHz	79.1	78.4	78.5	77.9	✓
4 KHz	76.7	75.8	76.7	76.1	✓
BACK SAVE RETEST					

Pass - Tick/Check mark (✓) The **NEW** and **OLD** (Stored) data for each of the two channels are within ± 3 dB and are within the absolute limits.

Query - Question mark (?) Values differ by more than ± 3 dB. The **NEW** and **OLD** levels are highlighted.

Fail - Cross (✗) Values are outside the absolute range. The **NEW** level only is highlighted.

The 1, 2 and 4kHz values may not be stored in the probe if a new probe is being used with the system. To save new data, run a Probe Test, record the values for each frequency and repeat by selecting **Retest**. Check that the values from two sequential tests are within ± 0.5 dB before selecting **Save**.


Save is only available to admin users. It is not available if the test was noisy or if the levels were outside the absolute range.

On selecting **Save**, the screen title **Overwrite Stored?** will be shown highlighted. Select **Yes** to save the new data or **No** to keep the current stored values which may be blank for a newly registered probe. Before entering Probe Test the user will be prompted to register the probe with the Otoport.

Select **Back** to exit the **Probe Test** screen and return to the **Configuration** screen.

17.2

ABR cable test

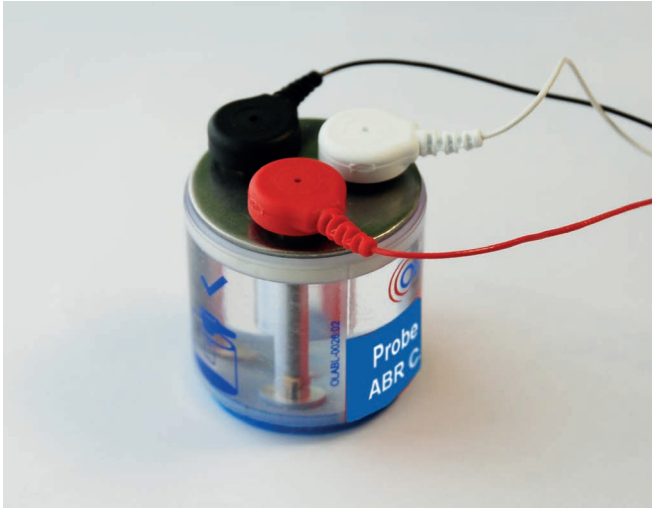

The ABR cable test checks the continuity of the electrode cables.

Attach the probe snaps to the top of the cable tester as illustrated.

Select **ABR Cable Test** and wait for the result to be displayed. If the electrode cables are OK then a large tick is displayed on the screen.

If any of the cables fail the test, a large cross is displayed.

Select **Details** to see the results for each cable. The impedances should show zero for all cables.

If any cable shows a cross, check that it is properly connected to the Otoport and retest. If it continues to fail then replace the cable.

17.3

Cavity test

Due to mechanical or electrical failure or a faulty probe, the system may itself produce signals during a test that have similar characteristics to an OAE response. The test cavity will not produce any OAE signal so any signal produced in the cavity is the result of a fault.

By performing an OAE test in a cavity rather than an ear it is possible to determine whether signal responses recorded in the ear are being generated by a fault.

Follow the instructions in **Probe test** for inserting the probe into the test cavity. Start a test on the Otoport as you would for an ordinary ear (see chapter 7 **OAE test selection**).

Follow the **Checkfit** and **Test** screen sequences until the test stops. In a cavity the Checkfit screen should indicate a large cavity volume.

If the result **Stopped Too Soon, Too Noisy** or **Poor Probe Fit** is achieved, retest checking that the probe ear piece is firmly inserted into the test cavity and that the noise conditions within the room are acceptable for a test to be conducted. Continue to retest until a **No Valid OAE** result is given.

At the end of the test:

1. Use the arrow keys to view the **data table** and check that the **noise** values are below -5 in all bands.
2. Use the arrows again to view the **Circles** screen and check that none of the circles contains a tick.

If either of these conditions is not met, save and retest. Make sure the earpiece has been firmly pressed into the test cavity.

Condition 1 will only be achieved with low environmental noise levels. If this is not achieved, continue to repeat the test in a quiet environment. Electromagnetic interference is an 'invisible' source of noise, so if there are persistent problems and other hardware issues have been eliminated, try to move to another location to perform the tests.

If condition 2 is NOT met during a repeat measurement, then check the top of the test cavity ensure that it is securely attached to the clear plastic part of the test cavity. If the resources are available repeat the test with a different test cavity and then with a different probe. This will identify which component is responsible for the problem. Contact your dealer or Otodynamics for further advice.

Note:

If a signal is detected in the test cavity, ensure that five successful cavity tests are performed on the Otoport before returning it to use. Refit the probe in the cavity between each test.

Cavity tests should be run using a DP and a TE test type. Use stimulus levels of 65-55 for the DP test.

17.4

Occlusion test

If the probe coupler is not fitted correctly, sound may leak between the probe loudspeaker and microphone. The **Occlusion Test** helps to check that the probe is assembled and is performing correctly.

To occlude the probe place a finger firmly over the end of the coupler tubes to block sound from being omitted from the ear piece and to prevent ambient noise from being read by the microphone. Then start a test as normal.


The **Checkfit** size bar should be off the scale to the right, indicating a very low sound level and **Check probe fit** should be displayed.

If so, the **Occlusion Test** has passed.

If not, check that the coupler is fitted to the probe correctly, making sure the coupler tube ends are fully occluded by a finger and that the environmental noise level is low. It may be necessary to change the coupler tubes. Repeat the test if necessary.

17.5

Real ear test

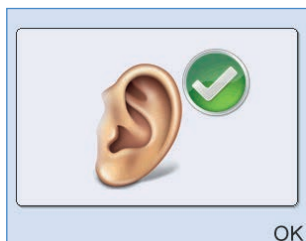

Testing with a known good ear allows for test data to be checked for reproducibility

Perform a test using the standard test procedure on the known good ear. This result may then be compared with previous results from the same ear. A Pass should be achieved (when pass bands are set to the default). Real ear tests should be performed in similar test environments to be comparable.

Real ear tests should be run in both DP High and TE Quick modes.

Some adult ears with no significant hearing loss produce little or no TEOAE. If possible the Real Ear Test should be performed on an ear which is known to have strong TEOAEs.

If you are unable to achieve a **Real Ear OK** result in an ear which is known to have OAEs then:

- Check the subject has no middle or outer ear problems, such as a cold or wax blockage, which might prevent OAE recording.
- Check a good probe fit has been achieved.
- Check that the probe is not blocked.
- Check the probe still passes the probe calibration test (see above).
- Try recording emissions from another subject.

If you are still unable to achieve a **Real Ear OK** result then, if the resources are available try recording with a different probe or with a different Otoport. If the problem persists, contact your dealer or Otodynamics.

18 Probe, tips and accessories

18.1 Probe and service accessories

Your kit will include a DPOAE probe with sample coupler tubes and spare probe body/lid. See chapter 2 **Equipment identification** for details.

18.2 Probe cable clip



The probe cable clip is provided to aid the practical aspects of positioning and securing the probe cable during OAE testing. Using the probe cable clip can improve your test times by reducing noise from cable rub and providing greater probe stability.

18.2.1 Using the cable clip

Push the plunger to open the cable grip.



Place the probe cable in the slot and release the plunger. The position of the clip on the cable can be adjusted if necessary.



Open the crocodile clothing clip.



Attach the probe cable clip to the patient's clothing.



If the cable slips through the grip, turn the head to grip the cable.

Use a sterile wipe to clean the clip.

18.3

DPOAE+TEOAE probe tips

 <p>R4.8S REF T-R4.8S Fits ~4.8mm ear canal Small newborns</p>	 <p>R5.8B REF T-R5.8B Fits ~5.8mm ear canal Most newborns</p>
 <p>R6.8B REF T-R6.8B Fits ~6.8mm ear canal Large newborns and first year infants</p>	 <p>R7M REF T-R7M Fits ~7mm ear canal Infants and children</p>
 <p>R8M REF T-R8M Fits ~8mm ear canal Infants and small adult ears</p>	 <p>R9M REF T-R9M Fits ~9mm ear canal Most adult ears</p>
 <p>R11M REF T-R11M Fits ~11mm ear canal Large adult ears</p>	 <p>R13M REF T-R13M Fits ~13mm ear canal Extra large adult ears</p>

Samples of each tip size are provided with your instrument. Further supplies may be obtained from your distributor or from Otodynamics.

18.3.1 Use of tips



All Otodynamics probe tips are disposable and **MUST** be discarded after each test. The probe coupler tubes should be visually examined for signs of contamination and the outer parts cleaned with an antiseptic wipe. Take care not to squeeze any cleaning fluid into the tubes.

OAEs should **NOT** be conducted if there is evidence of fluid of any kind in the ear canal. Not only does this pose a contamination risk, but OAEs cannot be recorded through fluid.

In the event of an accident with body fluids, the tip, coupler tubes and probe body must be changed.

19 Probe care



19.1 Cleaning

Otodynamics does not recommend the use of bleaches such as sodium hypochlorite based cleansers.

The following is the suggested method of cleaning an Otodynamics probe. It should be noted that the probe is a precision assembly and, as such, care should be taken throughout in its handling and cleaning.

Cable - The cable may be cleaned with alcohol based antiseptic fluid or wipes.

Probe casing - The probe casing may be cleaned using alcohol based antiseptic wipes and dried with a tissue immediately afterwards. Do not allow liquids to enter the sound tubes.

Coupler assembly - Each coupler assembly has two sound tubes. These are protected from ingress of foreign materials by wax guards in the tubes and by the disposable probe tip. There is a loudspeaker at the end of one tube and a microphone at the end of the other. Cleaning solution must not penetrate the tubes.


19.2 Changing probe coupler tubes



The probe has sound tubes combined into a single coupler assembly that can easily be replaced at regular intervals or when contaminated.


19.2.1 Disassembling the probe

First, unplug the probe from the instrument. Remove the tip and then the lid (fig. 1). Remove the coupler tubes by pushing the end of the tubes down onto a hard surface (fig. 2). Pull out the tubes by gripping them (fig. 3). Never remove them by pulling on the cable. Finally, pull the coupler tubes away from the probe (fig. 4).

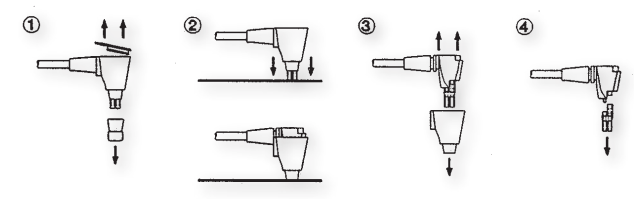

19.2.2 Reassembling the probe

Fit the new coupler tubes to the probe assembly (fig. 1). Fit the outer shell (figs. 2 and 3), followed by the lid (fig. 4). Click the lid into place using firm finger pressure only. Finally, fit a new tip (fig. 4).

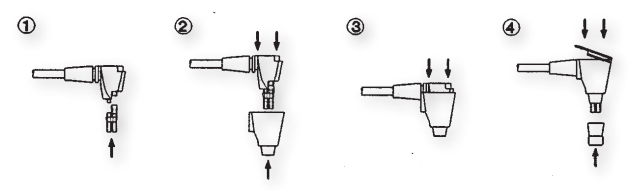

Illustrations show TPC (TEOAE) coupler tubes.

Notes:

- Fit a new tip for each test.
- Check that the coupler tubes are not contaminated before fitting the tip.
- If the coupler tubes are contaminated, **replace them**. We recommend fitting new coupler tubes at regular intervals (approx every 20-40 tests) as a preventive measure.
- Perform weekly probe QA tests (see chapter 17 **Quality checks**).

19.3

Probes safety note

Probes are designed for use with an Otodynamics disposable tip. Use of a tip is essential.

Use without a tip will expose the ear canal to the hard plastic sound tubes and this **might cause injury**.

Use without a tip or with an incorrect or non-Otodynamics tip may also cause serious errors in measurement. This could invalidate the OAE recording.



20 Care of the Otoport



The Otoport is robustly constructed but is a precision instrument, so should be handled with care. Be careful when connecting the probe, charger, PC cable or printer cable.

- Do not drop the Otoport
- Do not leave in strong sunlight
- Do not expose to high temperatures
- Do not touch the connector socket pins by hand
- Do not force the connection of the probe or charger/PC cable/printer cable
- Do not expose to moisture (keep it dry)

20.1

Use of the Otoport and cleaning

The following is a suggested cleaning method for the Otoport and probe. The Otoport and accessories are precision assemblies, so care should be taken throughout handling and cleaning.

Other than the probe ear piece and cable, the Otoport hardware should not come into contact with the patient being tested. Otodynamics probe tips are disposable and for single use only. A new tip should be used for each ear tested. The tip protrudes ~ 0.5mm beyond the end of the probe coupler, to prevent contact of the sound tubes with the patient.

Between patients, wipe the probe ear piece and cable with an alcohol based sterile wipe or cloth and antiseptic fluid. Dry the assembly with tissue immediately afterwards and do not let liquid pass down the coupler sound tubes. The probe ear piece is serviceable and its body, lid and coupler tubes can be replaced. The coupler tubes should be replaced weekly or after 20-40 tests, or if they have been contaminated. The body and lid should be replaced if contaminated. Visually check the ear piece for signs of dirt before each test.

Before fitting each tip, ensure the sound tubes are carefully examined for

any sign of debris that may have entered them. Replace any part of the probe ear piece as necessary. (See chapter 19 **Probe care** for details)

Ensure your hands are cleaned thoroughly between each patient tested.

Clean the Otoport each day before a testing session, or according to local requirements. Ensure the Otoport is cleaned if it becomes contaminated. Clean surfaces of the Otoport with an alcohol based sterile wipe or cloth and antiseptic fluid. Dry the Otoport with tissue immediately afterwards. Do not allow liquid to enter the instrument and do not immerse in fluid. Do not allow liquid to come into contact with the connection sockets. Do not poke any materials into either the probe or charger/pc cable sockets.

If additional hygienic protection is required, use the Otoport in an infection control sleeve. This can also be cleaned with a sterile wipe or cloth with antiseptic fluid. The sleeves are disposable, so should be replaced weekly or after approximately every 50 tests.

21 Power

Important Note:

Only charge your Otoport with the charger, charging cradle, or docking station supplied by Otodynamics

21.1 Battery life

The Otoport is powered using an internal rechargeable battery. The battery will provide enough power for over 250 OAE or 100 ABR tests from a single charge with a battery life of up to 8 hours. Note that the battery life depends on the Otoport usage pattern. With built in power save functions and by switching the device off for the periods between tests, the battery will provide enough power for over a week's intensive use.

21.2 Initial charge

The Otoport is fully charged before it leaves the Otodynamics factory. However, the battery will discharge slowly, even if the device is switched off. It is therefore recommended that an initial charge is provided to fully charge the battery before using your Otoport for the first time.

Standby

To save power, the Otoport will go into standby mode after 1.5 minutes of inactivity.

The Otoport will not go into standby if a test is being performed.

To resume from standby, press any button on the keypad. The Otoport will wake up and return to the previous screen displayed.

If the Otoport is left for 20 minutes in standby it will turn off. An audible beep will be emitted from the device for a period of 10 seconds to alert the user prior to the automatic shut down.


Notes:

Following an OAE recording, always save test data, as data that has not been saved prior to auto switch off will be lost.

Over time batteries will wear and lose their capacity, resulting in quicker discharge. The batteries may therefore need replacing around every 4 years of use.

21.4

Battery charge

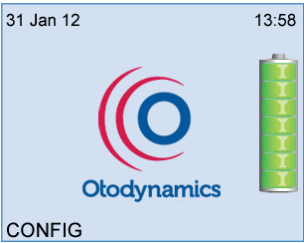


When the Otoport is switched on, the opening screen shows a battery indicator which displays the remaining level of battery charge.

The indicator has 5 segments which convey the total battery charge remaining. The battery segments are shaded according to the following criteria.

Segments Displayed	Battery Power (%)
7	95 - 100
6	75 - 94
5	55 - 74
4	40 - 54
3	30 - 39
2	20 - 29
1	10 - 19
0	< 10

21.4.1


Low battery

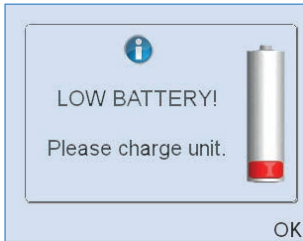

When the battery power reaches less than 10% remaining a **Low Battery** warning message will be displayed. This equates to approximately 30 minutes of testing time. Select **OK** to accept the message and return to the previous screen. This screen will continue to appear every minute, as a reminder to charge the battery.

21.4.2

Critical battery

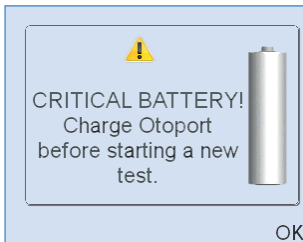

When the battery power reaches 7% remaining a **Critical Battery** warning message will appear on screen. This equates to approximately 10 minutes of use. Select **OK** to accept the message and return to the previous screen. It will not be possible to start a new test when the Otoport has reached this level of charge. The Otoport should be charged as soon as convenient.

21.4.3

Auto switch off

The Otoport will automatically switch off when the battery is empty. It will be necessary to charge the Otoport before it will switch on again.

21.5

Charging the Otoport



Observe the on-screen battery indicators to determine when to charge your Otoport. In general it is advisable to charge the Otoport batteries when the indicator is empty, showing less than 10% charge. However, the batteries should be at least 30% charged if a full day's testing is planned.

It is recommended to charge the Otoport using the charger supplied, but it is also possible to charge the device using the PC cable connected to a PC.

Note:

Do not charge more than one Otoport on the same PC at any one time.

21.5.1

Connecting the Otoport for charging

Switch off the Otoport prior to charging.

Connect the mains lead to the charger and plug the mains lead into a power socket and switch on the power. The green light on the charger will illuminate indicating it is powered.



Then connect the slotted charger plug to the Otoport. Ensure the arrow is facing upwards.



Notes:

If forced it is possible to insert the charger connector into the Otoport the wrong way up. In this position the Otoport will not charge.

Disconnect the connector and re-insert with the arrow facing upwards.



If the cables provided with your Otoport have a locking connector, as shown below, squeeze the release keys at the sides of the connector when removing the plug.



When the Otoport is connected the display will show the current battery level. This screen is updated every minute to show how the charge is progressing.

A full charge will take up to 4 ½ hours.

When the device is fully charged a large tick will appear on the screen.

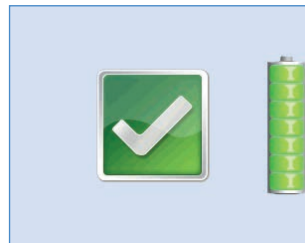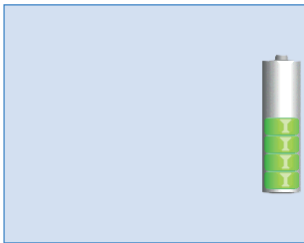

21.5.2

Additional charge indicators

There are additional charge indicators on the side of the Otoport.



- **Power light** - The green light below the plug symbol shows that the device is powered.
- **Charging light** - The orange light below the battery symbol will illuminate when the device is being charged.

Note:

If the device appears fully charged, with a tick displayed on screen, but the charging light is still on, if convenient, allow the device to continue to charge until the charge light goes out.

It is possible to leave the charger connected to the Otoport for extended periods, even if the device is fully charged. This may be convenient if you wish to leave the device charging overnight.

When powered by either a charger or PC, the Otoport is powered from the attached device and not its internal batteries.

When connected to a charger it is possible to switch on and control the Otoport but it is not possible to run a test.

When connected to a PC it is not possible to control the Otoport. If the Otoport is on when it is connected to a PC the current screen displayed will remain until the device is unplugged again.

21.5.3


Disconnecting the Otoport

When the charging cable is disconnected, the power light will extinguish on the Otoport and if the Otoport was off prior to the charging session, the screen will return to blank. If on during the charging session the current screen will remain displayed.



21.6

Conditioning the Otoport battery

In order maintain the Otoport batteries and keep them at optimal performance you should condition the battery once per year, or if the unit batteries appear to run down more quickly than expected. This process involves completely discharging the battery, using a function provided in the Otoport **System** area and then fully charging the device (see section 15.4 **System**).

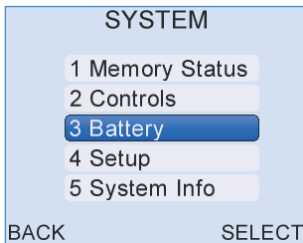

The condition utility is available from the **Configuration** menu by selecting **System** then **Battery**. Selecting **Condition** and confirming will set the device to full power to drain the battery.

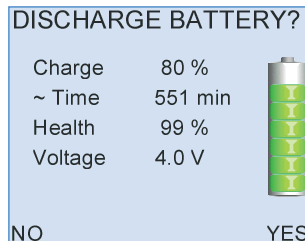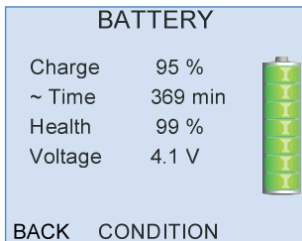

This process can take up to 6 hours. Select **Cancel** to stop the conditioning process. The Otoport will automatically switch off when the battery has been fully discharged. Now fully charge the Otoport to complete the battery condition cycle. Wait for the tick on the screen and for the charge light to extinguish, to confirm a full charge.

21.6.1

Additional battery care

If the Otoport is not in regular use, in order to maintain the battery, fully charge the device every two months.

21.7

Otoport OAE+ABR

The instrument is powered from the Otoport's internal rechargeable battery. The Otoport may be charged in situ via the **Charger and PC cable socket** at the lower end of the ABR Module.

21.7.1

Connecting the Otoport OAE+ABR to the charger cable

Switch off the instrument prior to charging.

Connect the mains lead to the charger, plug the mains lead into a power socket and switch on the power. The green light on the charger will illuminate indicating it is powered.

Then connect the slotted charger plug to the base of the instrument. Ensure the arrows are facing upwards.

21.7.2

Charge indicator lights

There are additional charge indicators on the side of the Otoport OAE+ABR.

- **Power light** - The green light above the plug symbol shows that the device is powered.
- **Charging light** - The orange light above the battery symbol will illuminate when the device is being charged.

22 Equipment troubleshooting

22.1 Otoport lock-up

In the unlikely event of an Otoport lock-up and it is not possible to control the device, turn the unit off and switch it on again. If this is not possible, hold down the **On/off** power button for 10 seconds; this will force the unit to switch off. Turn on the Otoport again.

22.2 Switch on

During switch on, the Otoport conducts a series of system checks. If the Otoport will not switch on and complete its start up sequence, check that it is charged and try again. If the Otoport still fails to complete its start up sequence then contact your distributor or Otodynamics for support.

22.3 System details

The **Configuration** area includes in the **System** menu a **System details** screen. This screen provides information for Otodynamics engineers relating to the Otoport hardware. If your device is not functioning correctly or you suspect a fault, go to the **System details** menu and check for any numbers reported at the top of the screen. For support regarding a fault, report code numbers to your dealer or Otodynamics.


Select **Reset** to reset the Otoport to factory default settings. Changes from the default setting and any users or worklist patients added to the device will be lost. No test data will be removed.

Select **Format** to reformat the Otoport database. Any records held on the device will be irrecoverably lost.

The **Format** and **Reset** options are only available to users with Admin rights.

22.4

Instrument fault message

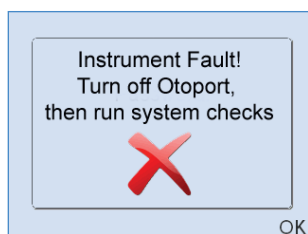

In the event of an instrument fault, the following message will be displayed at the start a test.

Instrument fault, turn off Otoport then run system checks.

No stimulus will be delivered from the Otoport Flexi probe and you will not be able to start a test. Turn off the device and then switch it on again.

Important note:

The **Instrument Fault** message can be triggered by a partially connected probe. Ensure that the probe is fully connected and the knurled sleeve screwed up correctly. (See **Connecting the probe** in the **Getting started** section).

Run the probe checks (see chapter 17). If the tests are 'OK' the device is functioning correctly and can be used for OAE testing again.

If you receive the **Instrument fault** message again, contact your dealer or Otodynamics for support.

Hardware fault messages

The Otoport performs a series of hardware tests when it is first turned on. In the event of a fault being detected the following message will be displayed:



The error code number displayed indicates the type of error detected. You should make a note of this error number. The Otoport should then be turned on and off a number of times to ensure that the error doesn't recur.

If you receive the hardware fault message again, contact your distributor or Otodynamics for support.

Error 2

An Error 2 message indicates that excessive noise was detected during start up. The noise may have been detected through the probe, if it was connected. Noise detected through the probe does not indicate a fault. If this message is displayed, turn the unit off, disconnect the probe and then turn it back on. If the message is consistently displayed with the probe disconnected, then contact Otodynamics.

23 Training

It is important that the operator of the Otoport is properly trained before using the instrument. The manual should be read before use and note taken of the sections marked with the training required symbol.



Where the training symbol is directly beneath a chapter title, it indicates that training is required for everything within the chapter. Where the symbol appears beneath a section heading, it indicates that training is required for that section only.

Where the device is to be used for other than the screening of healthy individuals, the user must be competent in the recognition of medical conditions associated with ears which may preclude testing (see **Contraindications**). Training for that purpose must be given by an audiologist or medical professional.

In all cases before application of the probe to the ear there must be an appropriate visual examination of the ear as specified by an audiologist or medical professional as part of training.

Training in operating the device is provided by Otodynamics Ltd in the UK. Training in the operation of the device elsewhere is via an approved dealer who has been trained by Otodynamics. Training on OAEs and use of the equipment may also be provided by previously trained staff and qualified audiologists.

Ensure your local policy for infection control is followed, as well as reading the recommendations in this manual (see section 20.1 **Use of the Otoport and cleaning**).

If a problem occurs during the operation of your Otoport or Otolink software or a message or warning appears that you don't understand, make note of the issue and messages provided. Refer these to your department lead, or directly to Otodynamics or your dealer for support.

Obtaining service

Otodynamics or its authorised distributor will replace or service, free of charge, this Otoport during the period of warranty, where the fault is not associated with misuse. Servicing after that period will be provided at reasonable cost.

Otodynamics highly recommends that the Otoport is serviced every three years (this is not a device safe operation requirement). During Otodynamics approved service the Otoport system will be thoroughly inspected and calibration will be checked; any system items with significant wear/tear or negatively affecting the system's calibration will be replaced at no additional charge.

The expected service life of the Otoport is ten years from the date of manufacture.

Probes failing because of faulty construction will be replaced subject to inspection. Probes must be treated with care. Do not allow cleaning fluid to enter the sound tubes.

When sending equipment to Otodynamics for service or repair, please ensure all items, particularly the OAE instrument and probe, are clean and free from contamination. Otodynamics cannot guarantee the equipment will be contamination free when returned to you and suggest that it is cleaned in accordance with your infection control protocols before being put back into use.

Please contact your distributor or Otodynamics for advice before returning an item for repair. You will be asked for your instrument serial number, which can be found on the back on the Otoport.



Otodynamics Ltd.
30-38 Beaconsfield Road
Hatfield
Hertfordshire AL10 8BB
UK

Tel: +44 1707 267540
Fax: +44 1707 262327
E-mail: support@otodynamics.com

www.otodynamics.com

25 Calibration

The Otoport is a precision instrument designed to make accurate measurements of OAE & ABR responses. Before it leaves Otodynamics, each system supplied is calibrated using high quality acoustic measuring equipment traceable to national standards.

Users should conduct the recommended weekly checks (see chapter 17) to ensure the instrument is working correctly. In addition to this, the calibration of the instrument should be periodically checked with laboratory equipment. Otodynamics advises regular calibration checks at intervals not exceeding 3 years and ideally annually.

The **About** screen displays the calibration due date for your Otoport, if a date has been set (see section 15.4.5). A prompt when switching on will warn that calibration is due from 30 days before the due date.

Contact your dealer or Otodynamics to arrange a calibration check.

26 Mode of operation

26.1 DPOAE test

Parameter	Description
Checkfit stimulus	80µs positive broadband square wave pulse with an intensity of 64dB pe (peak equivalent) in a 1cc cavity.
Sample rate	25.6kHz
Sample buffer	80ms (gives 2048 points)
FFT frequency bin	25Hz
DP Noise calculation	DP noise from the five spectral points above and the five points below the DP frequency. In the 'Rapid' noise mode, the mean of these points gives the noise level. In the 'Standard' noise mode the mean of these points plus two standard deviations gives the noise level.
Noise rejection calculation	The noise level for noise reject is calculated from the difference between consecutive 80ms samples.
Frequency ratio	$F2 = 1.22 F1$

26.2

TEOAE test

Parameter	Description
Stimulus	Idle 80µs positive broadband square wave pulse with an intensity of 64dB pe (peak equivalent) in a 1cc cavity.
	Adjusted 80µs positive broadband square wave.
	Test 300µs biphasic broadband triangular pulse.
Sample rate	20kHz
Stimulus pattern	
	Each sweep presents 8 stimuli responses with the stimulus presentation pattern: A A A B -A -A -A -B Where: B = -3A
Noise rejection calculation	
	The noise level for noise reject is calculated from the difference between consecutive sweeps.
Averaging	
	The responses from each stimuli in a sweep are summed and averaged. Averaging this stimulus pattern removes artefacts which scale linearly leaving only the OAE signal which is non linear. These sub averages are alternately added to two separate averages. These separate averages are referred to as waveforms A and B.

Signal and noise calculation

Measures of signal and noise levels are based on the correlation and differences between waveforms A and B.

Stimulus repetition rate

One stimulus every 13ms, approximately 80 stims per second.

Response window

2.5-12.5 ms or 4-10 ms after start of stimulus.
Cosine filtered with rise and fall time of 2ms

Response frequency bands

Half octave, centres at 1, 1.4, 2, 2.8 and 4kHz

Response frequency range

841-4757Hz

Microphone input filter

1189-4757Hz
The attenuation at these frequencies is 3dB.
Attenuation increases by 80dB/decade below and 40dB/decade above these frequencies.

Memory capacity

Patients	1000
Tests per patient	256
Total tests	1000

26.3


ABR test

Stimulus level	5-60 dBHL
Stimulus rate	51.8-57.9Hz
Stimulus polarity	Alternating
Stimulus type	Click or Chirp (see below)
Stimulus repetition rate	51.8-57.9 Hz
Evaluation method	Fsp & Template Correlation
Sampling rate	25.6 kHz
Frame length	17.3-18.8ms
Amplifier gain	75dB
Amplifier CMRR	> 60dB at 100 Hz
Input impedance	1M Ω 10 nF
Amplifier noise	20 nV / Hz @ 0.1-1 kHz
Input bandwidth	150-1000 Hz
Notch filter	None
Impedance sense Waveform	<p>For the measurment of impedance, the device delivers a 400Hz square wave giving in a worst-case (in to zero ohms) RMS current of <5uA with a <5uA DC component. The complete impedance measurement takes 2-3 seconds and consists of four bursts of 400Hz square wave. The first burst is 0-700mS long and the following three are 300-700mS long.</p> <p>Additionally, there are transient currents produced at device switch on and shut down. These have a peak current of less than 100uA with a duration of less than 0.5 secs.</p>
Impedence test range	0 to 99 k Ω


Display	EEG-level, ABR detection probability
Electrodes	Disposable wet gel electrodes (FDA 510(k) cleared)
Electrode Montage	
Positive electrode	Forehead
Negative electrode	Ipsilateral mastoid or nape of neck
Common electrode	Back of shoulder, cheek, or contralateral mastoid

26.3.1

Stimuli description

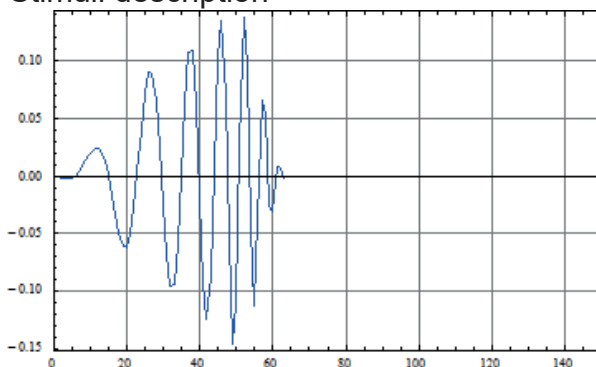

Click stimuli: 80 μ S duration square pulse of alternating polarity.

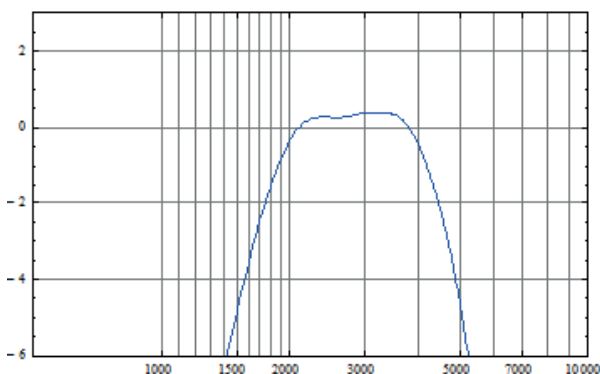

Chirp stimuli: 2.5ms duration rapidly swept tone of alternating polarity. The frequency dispersion of the chirp is defined by the delay at frequency $T(f) = k * f^{-d}$ with $k=0.0920$, and $d=0.4356$.

The wide band chirp waveform was cosine filtered in the time domain to give the required duration and a frequency range of 1686 to 4614Hz (-3dB points). The waveform and spectra of the short chirp are illustrated below.

Short Chirp time domain (x-axis in samples at 25.6kHz):

Short Chirp frequency domain:

26.3.2

Hearing Level determination

The hearing threshold for these stimuli was determined in a group of 20 subjects with normal hearing aged <25. The peak-to-peak levels (dBppSPL) of these stimuli were measured in a Brüel & Kjær Ear Simulator Type 4157. For short duration stimuli the dBppSPL values are always much higher than their dBHL value. For the Click dBppSPL in the ear simulator exceeds Otoport dBHL value by 33.6dB. For the Chirp dBppSPL in the ear simulator exceeds Otoport dBHL value by 29.5dB.

26.3.3

Screening test sensitivity

The 'sensitivity' of a hearing screener relates to the ability of the device to detect ears with hearing loss (i.e., the true positive detection rate). Sensitivity is measured as the probability of a 'No Valid response' result being correctly reported by the device when no response is actually present. Departure from the desired 100% sensitivity figure would indicate a false passes caused by the device misinterpreting electrical noise (biological and/or environmental) as a true response. This must be avoided even at the expense of unnecessarily referring some patients with normal hearing.

The sensitivity of a device is best measured with the screening device operating in its screening test mode in a real screening environment and exposed to all the differing levels of interfering noise in which the device can be used (e.g., EEG noise and power line interference of ABR and acoustic noise for OAEs). But crucially without any real response actually being present, this is achieved by not supplying any stimulus during the test.

It is important to note that the measured sensitivity of an instrument relates to the outcome of tests where there was definitely no response is present. When there is a hearing loss, we can assume that no ABR is present

below a certain stimulus level at which a clear response IS detectable in most normal healthy ears. This demonstrated measurement of Otoports sensitivity therefore only applies to the detection of hearing losses greater than a specific amount. It is the applied stimulus level that determines what range of hearing losses that will be detectable and to which the sensitivity figure applies.

For example, if the patients hearing is only slightly impaired and the stimulus level is adequate then a true response may still be recorded.

It is therefore recommended that the stimulus level is set to the lowest value which delivers the sensitivity required consistent with a manageable false positive rate. Stimulus levels between 35 and 40dBHL have been found appropriate on the Otoport ABR, with the 40dBHL level giving both high sensitivity to mild losses and low false positive results.

Sensitivity of the Otoport OAE+ABR for ABR screening

The sensitivity of the Otoport OAE+ABR for ABR hearing screening was measured using 349 recordings from 30 neonates (3 days to 4 weeks old). For the purpose of determining sensitivity to hearing loss in a realist screening environment with infants, the test was conducted with no stimulus delivered to the babies. All had passed an actual screening tests, but the absence of any stimulation meant there could be no true response present during the sensitivity test. A clear response would indicate to the possibility of missing an impaired ear.

For the experiment the instrument was configured to generate its default short chirp stimulation at a level of 35dBnHL at the default repetition rate for 50Hz powerline environments. However, the stimulating probe was fitted to a closed cavity near to the baby's ear, but so that no sound entered the ear and so no ABR was actually generated by the baby. The real-time electrical signals received by the Otoport from the electrodes on the baby were digitally recorded through the device for many minutes to collect a large amount of real EEG and EMG signals. These electrode signals were then replayed at their original level back into the Otoport OAE+ABR and a total of 3257 virtual ABR further tests run. This procedure ensured that the instrument was exposed all possible statistical combinations of noise and instrument timings. Each of the 3257 ABR test results were evaluated by each of the four pass criteria (PC1-4) of the Otoport ABR. The results below describe the rate of false (artefactual) passes obtained in when a realistically wide range of neonate electrode noise signals (i.e., from sleeping to restless) is processed by the device. As no acoustic stimulation

actually reached the ear, no real ABR was present, so all ‘passes’ are false. This data shows that the sensitivity of the Otoport ABR is between 99.79% and 99.94%, which is very good.

Very high sensitivity of the instrument is demonstrated with each pass criteria. Pass criteria PC2 and PC3 showed the highest sensitivity, exceeding 99.9%. This would be expected because PC2 and PC3 require that the response correlates with the neonate ABR template. PC1 and PC4 only require that an Fsp statistical criteria is met and so showed a slightly lower sensitivity of 99.79%.

Since the acoustic stimulus was not delivered to the ear, this sensitivity data is valid for all stimulus settings and levels up to a level where electrical artefacts from the probe might create an artefactual pass. Rigorous tests showed that no artefactual passes occurred due to electrical stimulus artefacts up to the maximum stimulus level of the instrument, for both click and short chirp stimuli.

	Pass Criteria			
	PC1	PC2	PC3	PC4
Tests	3257	3257	3257	3257
Passes	7	2	2	7
Pass probability (%)	0.21	0.06	0.06	0.21
CI(Hi) (%)	0.44	0.22	0.22	0.44
CI(Low) (%)	0.09	0.01	0.01	0.09
Sensitivity (1 - Pass prob)	99.79%	99.94%	99.94%	99.79%

Confidence Interval (CI) measurements are given at 95%.

26.3.4

ABR test specificity

The specificity of an ABR hearing screening instrument quantifies the ability of the device to identify ears with normal hearing (the true negative rate). When there is no hearing loss, we can assume that an ABR is present. 'Specificity' is the probability of a 'Valid ABR', (a pass), result when an ABR is truly present. In practice, patient and environmental noise can obscure a true ABR response. This means that in practice ABR screening test specificity is variable and dependent on both the size of the individuals ABR at the electrodes and the levels of noise occurring during the test. Both vary according to the individual, electrode connection, position, resting state of the infant and the environment.

To determine specificity the mean ABR amplitudes from 270 infants was determined from healthy normally hearing baby's ABR recorded by the Otoport OAE+ABR using our short chirp stimulus at a level of 35dBnHL at the default repetition rate. The noise levels recorded by the Otoport OAE+ABR instrument during tests when the baby was considered quiet enough to test, were averaged, to give a realistic benchmark noise level against which ABRs must be detected.

To supplement the measurement of ABR amplitudes seen on the Otoport we incorporated range (i.e., the spread) of ABR amplitudes determined by an historic controlled study of 3200 infant ABR recordings at 30dBHL*. This helped determine the probability of there being exceptionally small ABR amplitude from normal ear, not captured in our smaller 270 infant trial.

Using this data and applying the Pass Criteria built into the Otoport OAE+ABR, we determined the probability of the Otoport OAE+ABR identifying the ABRs present in the normal population. This included the correct proportion of the weakest ABRs present on the normal population detectable against fluctuating noise based on the average amplitude present in 'quiet' babies. This provided a robust measure of specificity. Results are shown in the table below:

	All Pass Criteria
Pass probability (%)	99.70
CI(Hi) (%)	99.75
CI(Low) (%)	99.59
Specificity	99.79%

Important Notes:

- High EEG, myogenic or powerline noise levels can greatly reduce specificity.
- Testing with active infants will reduce specificity, depending on the movement noise.
- Testing with higher stimulus levels will increase specificity because the response will be larger but will reduce the range of threshold elevations to which the instrument is sensitive (according to the stimulus dBnHL used).
- Using 40dB HL stimulation instead of 35dBHL will increase specificity and decrease sensitivity to only slight hearing losses while maintaining sensitivity to mild losses. Using lower than 35dB HL stimulation will further decrease specificity and increase sensitivity to slight hearing losses.
- Testing with a 60Hz powerline setting rather than 50Hz will have an no significant effect on specificity since the ABR response size change is minimal between 50 and 60 Hz stimulus rates (Less than 1dB).
- Testing with a click stimulus rather than our short chirp will slightly decrease specificity because click stimuli generate a slightly smaller ABR response than a chirp of identical hearing level (due to reduced synchronisation). The typical ABR amplitude reduction for clicks relative to short chirps is of the order of 3dB for near threshold stimulation. This translates to a decrease in specificity to 98.6% with click stimuli.

*Norton, SJ, Gorga M P, Widen, JE, Folsom, RC, Sininger, YS, Cone-Wesson, B, Vohr, BR and Fletcher, KA. Identification of Neonatal Hearing Impairment: Summary and Recommendations, Ear & Hearing, 21:5, pp 529-535, 2000

27 Technical specifications

27.1 Otoport

Note:

The Otoport/Otocheck has no user serviceable parts. Any required servicing must be conducted by Otodynamics Ltd or authorised service facilities only

27.1.1 Physical

Hand-held device: 197mm x 70mm (max) x 30mm
Weight 0.55lbs (250g)
Charger: 90mm x 38mm x 28mm – Weight 120g

27.1.2 Interfaces

Probe connector compatible with Otodynamics UGx probes (8 pin)
Charging/Data connector - connects to Otodynamics PSU (charging) or to PC USB port (USB 1.1 or 2.0) via Data Cable
Bluetooth wireless print (option)

27.1.3 Indicators

Data Display: Resolution: QVGA (320 x 240 pixels), 166 dpi
Technology: Colour LCD, 16 bit (displaying 65K colours)
Viewable Area: 46.5mm x 36.5mm
Backlight: White - intelligent control
Probe fit: Noise OK: Blue LED ('N')
Stimulus OK: Blue LED ('S')
Power/Charge: Power OK: Green LED
Fast charge: Amber LED
Audible: Wide range speaker provides audio feedback of status

27.1.4 Keypad

19 key alphanumeric with cursor control and soft keys

27.1.5 Clock/Calendar

Internal Real Time Clock/Calendar operates to 2099

27.1.6

Power

Li-Polymer Battery
Intelligent multi-level power control for charging/testing/idle/sleep/shutdown:
After 1.5 minutes unit will enter sleep mode
After 20 minutes in sleep mode unit will shut down
Sleep time: 20 hours minimum (with fully charged battery)
Running time: 6 hours minimum (continuous data collection)
Battery voltage
operating range: 3-4.2V
Max consumption
when testing: 1W (Otoport) or 1.3W (Otoport ABR)
Max consumption
when charging: 2.5W
Source: 1000mAh lithium polymer internal rechargeable cells
Charge time: 3 hours to 90% capacity
Approximately 4 hours to 100%

27.1.7

Hardware Option

Bluetooth wireless technology enabled printing

27.1.8

Hardware processing and storage

Embedded microcontroller plus dedicated hardware DSP engine
4GB of non-volatile memory for storing programs, configuration, patient details and test results

27.1.9

Analogue performance

Output channels: 2 x 16bit resolution
Input channels: 1 x 16bit resolution
Sample rate: Variable
Frequency response: Electrical – 160Hz to 12KHz

27.1.10

Accuracy

The Otoport measures the sound delivered to the ear as a stimulus and automatically adjusts its level to be equal to the nominal value set. This ‘in-the-ear’ calibration process compensates for different ear canal sizes. It is most effective below 3kHz. Above this frequency sound levels may depart slightly from nominal due to individual ear acoustics. The device complies with the relevant standard (60645-6:2010 - 5.3.3) which requires that in a standard ear simulator/coupler any inaccuracy in stimulation level must not exceed $\pm 3\text{dB}$ for frequencies up to 4kHz or $\pm 5\text{dB}$ for frequencies above 4kHz.

Our OAE probe contains a microphone which is used to both calibrate the stimulus sound level and detect the otoacoustic emission. This ensures that the same accuracy applies to both applied stimulus and the recorded OAE sound levels. All our probes are factory tested and calibrated to be within these limits.

27.1.11

Environmental



Protect from heat and radioactive sources



Keep dry

If the environment changes rapidly in temperature, humidity/pressure environments do not use the device for six hours following the change.

Transport and storage:



Temperature range: 0 to 40 Celsius



Pressure: 23KPa to 120KPa



Humidity: 10% to 90% non-condensing

Protect Otoport Product from heat and radioactive sources
Keep Otoport Product dry

Operation:



Indoor use

Temperature range: 5 to 40 Celsius

Normal atmospheric pressure conditions with extremes in the range of 80-120kPa *



Relative Humidity: Noncondensing: 10% to 90%

Warm-up time: <10s when unit is stored within stated temperature range

*Otodynamics instruments and probes are calibrated at an ambient pressure of 101kPa (standard atmospheric pressure at sea level). Lowering the ambient pressure significantly (e.g. when operating at altitude) alters the acoustic response of the probe. For instance, at an ambient pressure of 80 kPa (standard atmospheric pressure at 2000m) changes of up to 2 dB can be observed in the response of the probe around 2KHz. This could cause the probe to fail standard calibration tests.

The Otoport Medical Device is not intended to operate in oxygen rich environments and is not to be used in conjunction with flammable agent.

27.1.12

Classifications and standards

Device Classification:

Class IIa under rules 5 and 10 of Medical Device Directive [93/42/EEC] & [MEDDEV 2. 4/1 Rev. 9].

The Otoport and Otoport+ABR products are declared to be in compliance with the council directives 93/42/EEC Annex II (excluding Section 4), 93/68/EEC, 2001/104/EC and 2007/47/EC and new Regulation (EU) 2017/745 of 5 April 2017 on medical devices at the product level (taking account of the intended purpose of the devices concerned).

In addition, the Otoport and Otoport+ABR meet the requirements of the Registration, Evaluation, Authorisation and Restriction of Chemicals - REACH Regulation (EC) No 440/2008 and (EC) No 1907/2006; of the Waste Electrical & Electronic Equipment - WEEE Directive 2012/19/EU; and of the Restriction of Hazardous Substances - RoHS Directive 2011/65/EU and Packaging / Packaging Waste Directive 94/62/EC.

Declared Conformity:

Otoport and Otoport+ABR products do not contain any of the restricted substances in concentrations and applications not permitted by the RoHS Directive (maximum concentration values tolerated by weight in homogeneous materials):

- Cadmium (Cd- 0.01 %); Lead (Pb – 0.1 %); Hexavalent Chromium (Cr6+- 0.1 %); Mercury (Hg- 0.1 %);

PBB's (Polybrominated biphenyls) (PBB- 0.1 %); PBDE's (Polybrominated diphenyl ethers) (PBDE 0.1 %);

- Adaptation of RoHS Directive issued (2015/863/EU) for the four additional phthalate substances:

Bis (2-ethylhexyl) phthalate (DEHP – 0.1%); Butyl benzyl phthalate (BBP – 0.1%); Dibutyl phthalate (DBP – 0.1%);

Diisobutyl phthalate (DIBP – 0.1%). Otodynamics Otoport and Otoport+ABR products do not contain phthalates.

- No Ozone Depleting Substances are used by Otodynamics / its Products.

- None of the following are used by Otodynamics in its Products: Polychlorinated Biphenyls (PCBs); Chlorinated Paraffins; brominated flame retardants, asbestos, chlorofluorocarbons (CFC's), hydrochlorofluorocarbons (HCFC's), hydrofluorocarbons (HFC's), Tributyl Tin (TBT); Triphenyl Tin (TPT) and Tributyl Tin Oxide (TBTO).
- Otodynamics products do not contain Latex and do not contain Materials Derived from Animal Sources.
- Materials used in the manufacturing processes for the Otodynamics products are not Substances of Very High Concern (SVHC) and are in line with REACH regulations.
- Otoport and Otoport+ABR packaging is recyclable.
- The Otoport and Otoport+ABR medical device / system is not supplied sterile or intended to be sterilized by the user. It is recommended that probe tips, electrodes and ear cups are for SINGLE PATIENT use only.

Otoport and Otoport+ABR Declared Conformance relating to the following above and other standards:

RoHS / Other: EN 50581:2012; EN 50419:2006; EN 60601-1-9:2008+A1:2013; EN ISO 14001:2015; ISO 14040: 2006; EN ISO 10993-1:2009/AC:2010.

QMS: EN ISO 13485:2016 & EN ISO 14971: 2012.

Safety: EN 60601-1:2006+ A12:2014; EN 60601-1-6:2010+ A1:2015; EN 62366-1:2015; EN 60601-2-40:1998 (IEC 60601-2-40:2016); EN 62304: 2006+ A1:2015. IEC 60601-1:2005+A1:2012, CAN/CSA-C22.2 No. 60601-1:14, ANSI/AAMI ES60601-1: 2005(R) 2012, UL 60601-1 and KS C IEC 60601-1.

EMC: EN 60601-1-2:2015; IEC 60601-1-2:2014, ed. 4.0; ETSI EN 301 489-17 V3.2.0; ETSI EN 301 489-1 V2.2.0

Other: EN 60645-3:2007; EN 60645-6:2010; EN 60645-7:2010; EN 50419:2006; EN ISO/IEC 17050-1:2010; EN 1041:2008+ A1:2013; EN ISO 15223-1:2016; EN ISO 14155:2011; ISO/IEC 27001:2013; EN ISO 27799:2016; ISO/IEC 27032:2012.

Note: The Otoport and Otoport+ABR products' Declaration of Conformity (DoC) can be provided on request.

27.2

Electromagnetic compatibility - User Guidance

The Otoport has been tested and certified to the medical electromagnetic compatibility standard EN 60601-1-2:2015. This standard limits both: the electromagnetic emissions generated by the Otoport; and the susceptibility of the Otoport to electromagnetic disturbances at the levels found in its intended environment.

In order that the instrument operates safely it should be put into service according to the Electromagnetic Compatibility (EMC) information provided here.

27.2.1

Suitable environments for operation

The Otoport is designed for use in a professional healthcare facility only. It must not be used near high frequency (HF) surgical equipment or in the Radio Frequency (RF) shielded room of medical equipment systems for magnetic resonance imaging.

27.2.2

Essential performance

Electromagnetic (EM) immunity of this Otoport was tested by exposing it to the EM disturbances detailed in the medical EMC standard EN 60601-1-2:2015. These EM disturbances are the maximum level normally expected in the Otoport's specified operating environment. During these tests the Otoport was shown to:

- (i) not indicate a 'PASS' result when a stimulus is applied but there is no physiological response to the stimulus;
- (ii) remain electrically safe;

In higher levels of EM disturbance than tested for, or for different types of EM disturbance, the user can expect to see increasingly large proportions of measurement data rejected. However, for reasonably foreseeable levels of EM disturbance it is improbable that electrical safety is compromised or that damaging levels of sound are generated. In these circumstances the increased rejection rate, and the operation of the detection algorithms, will ensure probability of falsely detecting a false OAE or ABR will not increase. However, at very high levels it will become impossible to record any data. If this occurs, you are advised to reduce or move away from the source of the EM disturbance.

Warning

Use of this equipment adjacent to or stacked with other equipment should be avoided because it could result in improper operation. If such use is necessary, this equipment and other equipment should be observed to verify that they are operating normally.

27.2.4

Cables that may affect electromagnetic compatibility

To ensure electromagnetic compatibility this equipment should only be used with the following cables:

- (i) UGD or UGS probe, as supplied by Otodynamics;
- (ii) charger and mains lead, as supplied Otodynamics;
- (iii) PC download cable, as supplied by Otodynamics;
- (iv) electrode cables, as supplied by Otodynamics or equivalent. Maximum length 2m.

Warning

Use of accessories, transducers and cables other than those specified or provided by Otodynamics could result in increased electromagnetic emissions or decreased electromagnetic immunity of this equipment and result in improper operation.

Warning

Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30cm (12 inches) to any part of the Otoport including cables specified by the manufacturer. Otherwise, degradation of the performance of this instrument could result.

27.3

Electromagnetic compatibility - Technical Description

27.3.1

Compliance levels

The Otoport has been tested and certified to the medical electromagnetic compatibility standard EN 60601-1-2:2015. Compliance levels are as below:

- (i) Electromagnetic emissions - complies with:

CISPR 11:2015

EC 61000-2:2014

IEC 61000-3:2013

The instrument is group 1, class B for the purposes of CISPR 11. Radio emissions limits are as given in tables 4 and 7 of CISPR 11:2015.

- (ii) Electromagnetic immunity - complies with:

IEC 61000-4-2:2008

IEC 61000-4-3:2013 + amendment 1:2007 + amendment 2:2010

IEC 61000-4-4:2012

IEC 61000-4-5:2014

IEC 61000-4-6:2013

IEC 61000-4-8:2009

IEC 61000-4-11:2004 + amendment 1:2017

All immunity test levels as in tables 4 to 9 of IEC 60601-1-2:2014 for medical EMC testing. The 'professional healthcare facility environment' immunity levels apply.

27.3.2

Deviations from the standard

The Otoport shows no deviations from the EN 60601-1-2:2015 EMC standard.

27.3.3

Maintaining essential performance for the expected service life

No special measures need to be taken to maintain basic safety and essential performance with regard to electromagnetic disturbances for the device's expected service life.

27.3.4

Details of radio receivers

The instrument contains the following intentional RF receivers:

- (i) **Bluetooth® receiver.** Operates in frequency range of 2.4000-2.4835GHz with a bandwidth of 1MHz hopping pseudo-randomly in the frequency range.
- (ii) **RFID.** Operates at 13.56MHz. ETSI EN 300-330-1 defines a transmit mask that is -65dB down at ± 0.9 Mhz from the carrier. Therefore the -65dB bandwidth is 1.8Mhz.

27.3.5

Details of radio transmitters

The instrument contains the following RF transmitters:

- (i) **Bluetooth®.** Operates in frequency range of 2.4000-2.4835GHz with a bandwidth of 1MHz hopping pseudo-randomly in the frequency range. The maximum radiated power is 20dBm. The modulation is Gaussian frequency shift keying or phase shift keying.
- (ii) **RFID.** Operates at 13.56MHz. ETSI EN 300-330-1 defines a transmit mask that is -65dB down at ± 0.9 Mhz from the carrier. Therefore the -65dB bandwidth is 1.8Mhz. The effective radiated power is not meaningful as this is a near field device. The maximum magnetic field generated is 60dB re uA/m. The modulation is amplitude shift keying.

27.3.6

Specific Absorption Rate SAR

The SAR is a measure of the rate at which radio frequency (RF) energy is absorbed by the human body.

27.3.7

RF Exposure

The Otoport / Bluetooth® technology complies with CE/FCC/IC RF exposure limits for general population / uncontrolled exposure. The Bluetooth® module “WT11i” or “WT11u” in Otoport and Otoport+ABR devices comply with SAR regulatory requirements. Otoport and Otoport+ABR can be used as hand-held devices with the WT11i or WT11u Bluetooth® module with the current antenna position of 8mm from the edge of the Otoport case and firmware setting output power level to 13dBm. Measurements confirm that the Otoport and Otoport+ABR maximum RF Energy output is below the limits set forth for CE, FCC and IC compliance.

Regional Standards

Europe

Radio Equipment Directive (2014/53/EU)

CE marking certification

Silicon Labs Declaration of Conformity - DoC for WT11i and WT11u.

Otodynamics Otoport and Otoport+ABR 3rd Body Test House Validation Safety & EMC measurements.

The WT11u is Bluetooth® qualified and the declaration ID is B016141 (QDID 22298).

SIG Listing

The Bluetooth® - SIG, Declaration ID: D034915.

US

Federal Communication Commission (FCC)

This device complies with Part 15 of the FCC rules. Operation is subject to the following two conditions. (1) This device may not cause harmful interference. (2) This device must accept any interference received, including interference that may cause undesired operation.

FCC ID for WT11i Bluetooth® - module currently used for Otoport / Otocheck USA: QOQWT11

FCC ID for WT11u Bluetooth® module alternative/future use for Otoport / Otocheck USA: QOQWT11U.

Canada

Industry Canada (IC)

This radio transmitter (IC: 5123A-WT11U) has been approved by Industry Canada to operate with the embedded chip antenna. Other antenna types are strictly prohibited for use with this device. This device complies with Industry Canada's license-exempt RSS standards. Operation is subject to the following two conditions. (1) This device may not cause interference. (2) This device must accept any interference, including interference that may cause undesired operation of the device.

Japan

MIC Japan

The WT11u module is certified for Japan. Certification number: 209-J00232 Since September 1, 2014.

EN60645-3 conformance notes

These notes are provided in compliance with EN60645-3 "Electroacoustics audiometric equipment - Part 3: test signals of short duration."

(a) Types of short duration stimuli:

The Otoport TEOAE test uses short duration stimuli. During test setup a 'rectangular stimulus' is used. During data collection a 'bipolar stimulus' is used. The rectangular is a unipolar pulse of 78uS length. The bipolar stimulus is 1 cycle of a triangle waveform of 240uS period. Both stimuli are low pass filtered by a 10kHz anti-alias filter, which 'rounds' any 'sharp edges'.

(b) Transducers and headband force:

The stimulus is delivered to the patient's ear using a UGS or UGD Otodynamics probe. The probe tip holds the probe ear piece in the ear canal, with no headband or other retaining device required.

(c) Sound field system:

The sound field is generated by the probe sealed in the ear canal by its tip.

(d & e) Calibration cavity and measurement type:

For the purposes of EN60645-3 calibration was performed in an occluded ear canal simulator conforming to IEC 60711 (Bruel and Kjaer type 4157). The probe was mounted in a DB2012 adaptor using an Otodynamics probe tip. The sound ports of the probe were aligned with the 4157 reference plane. A UGD probe was used for the calibration. Sound levels from the 4157 ear simulator were measured in dB SPL peak-to-peak equivalent, as defined in EN60645-3.

(f) Signal levels:

The following conversion factors convert between the stimulus level reported on the Otoport screen and the signal level in the IEC 60711 occluded ear simulator:

rectangular stimulus: -6.1dB

bipolar stimulus: -7.1dB

The following conversion factors convert between the signal level generated in the ear simulator by the Otoport stimulus and the level that would be generated by a 'reference stimulus' of the same peak to peak electrical drive. (The 'reference stimulus is a 100uS unipolar rectangular pulse, as defined in EN60645-3.):

rectangular stimulus: +3.0dB

bipolar stimulus: +2.4dB

Suppose, for example, that a stimulus level of 90dB is reported by the Otoport during stimulus setup (rectangular stimulus). If this stimulus was replaced by the reference stimulus, of the same amplitude, the level generated in a IEC 60711 ear simulator would be:

$$90\text{dB} + -6.1\text{dB} + 3.0\text{dB} = 86.9 \text{ dB SPL peak-to-peak equivalent.}$$

(g) Polarity of stimulus:

The polarity of the stimulus varies between positive and negative, according to the TEOAE test sequence.

(h) Repetition rate:

The stimulus is repeated every 12.5mS during standard Otoport TEOAE setup and testing.

(i) Covered in (a) above

(j) Covered in (f) above

27.5

ABR Module

Note:

The ABR Module has no user serviceable parts. Any required servicing must be conducted by Otodynamics Ltd or authorised service facilities only.

27.5.1

Physical

Hand-held module: 278mm x 84mm x 38mm
Weight: 240g (490g with Otoport fitted)

27.5.2

Interfaces

Probe connectors compatible with Otodynamics UGS and UGD probes (8 pin)
Electrode connectors compatible with 1.5mm 'Touchproof' DIN 42-802 connectors
Charging/Data connector - connects to Otodynamics PSU (charging) or to PC USB port (USB 1.1 or 2.0) via Data Cable

27.5.3

Indicators

Data display:	Data is displayed via Otoport
Probe Fit:	Indicators on Otoport: Noise OK - Blue LED ('N') Stimulus OK - Blue LED ('S')
Impedance check:	Impedance OK - Green LED (one for each electrode socket)
Power/Charge:	Power OK - Green LED
Fast charge:	Amber LED
Audible:	Audio feedback via Otoport speaker

27.6

End of life management

The Otoport/ABR meets the requirements of the Waste Electrical & Electronic Equipment- WEEE Directive 2012/19/EU; and of the Restriction of Hazardous Substances- RoHS Directive 2011/65/EU and of Packaging/ Packaging Waste Directive 94/62/EC.



















When the Otoport product is discarded, the item must be sent to separate collection facilities for recovery and recycling.

- No hazardous materials are included in the Otoport/ABR.
- No Ozone Depleting Substances are used by the Otoport/ABR.
- No Latex is included in the Otoport/ABR. The Otoport/ABR does not contain any phthalates.
- Local guidance for disposal of medical devices should be followed, for example in the UK follow the NHS Healthcare (clinical) Waste National guidelines.
- When sending Otoport/ABR equipment that is no longer required for disposal, please ensure all items, particularly the instrument and probe(s)/ cables, are clean and free from contamination (cleaned in accordance with your infection control protocols).
- Prior to battery recycling, handling precautions and prohibitions for Li Ion Batteries must be read and understood. Follow VARTA Handling and Safety Precautions for Lilon & LiPolymer batteries.
- Otoport/ABR shipping package is recyclable; the Otoport/ABR is recyclable (Electronic Waste Recycling/ Plastics recycling); Battery Recycling
- In some territories, total waste management solutions are available and should be used for the the Otoport/ABR and accessories; these allow nationwide collection service and a sustainable licensed recycling solution with full traceability. Otherwise, all electrical and electronic products, batteries, and accumulators must be taken to separate collection facilities at the end of their working life. This requirement applies in the European Union.
- Do not dispose of these products as unsorted municipal waste.
- You can return your device and accessories to Otodynamics, or to any Otodynamics supplier.
- You can also contact your local authorities for advice on disposal.

27.7

Symbol explanations

Symbol	Description
	Class II
	Type BF
	Bluetooth® enabled
	Caution
	USB 1.1
	When discarded, the item must be sent to separate collection facilities for recovery and recycling
	Probe socket
	Battery charging indicator
	Power supply connection
S	Stimulus OK indicator
N	Noise OK indicator

Symbol	Description
	Refer to operating instructions
	Otodynamics' factory address
	Product catalogue number
	Product date of manufacture
	Product serial number
	RF transmitter
	Training required

28 Index

A

ABR 57
 ABR cable test 175
 ABR controls 30
 ABR module 34, 196, 225
 ABRScreen 139
 ABR test problems 64
 ABR test procedure 92
 Accuracy 214
 Adjusting 82
 Analogue performance 214
 Arrow (navigation) buttons 44
 Assembling the ABR Module with an
 Otoport 34
 Atypical waveform 104
 Auditory Brainstem Response 18
 Auto send 151
 Auto switch off 191

B

Backlight 47, 148
 Battery 52, 149, 188, 190
 Beep 80, 89
 Bilateral ABR testing 105
 Blue LEDs 47
 Bluetooth 150, 156, 221
 Bluetooth® 28
 Bluetooth wireless printing and
 download 156
 Brightness 148

C

Cable clip 179
 Cables 219
 Calendar 213
 Calibration 202
 Cancelling the test 80, 90
 Caution 13
 Cavity test 176
 Certification 29, 33
 Changing probe coupler tubes 183
 Charger and PC cable socket 26
 Charging status indicators 26
 Charging the Otoport 192
 Charging the printer 167
 Checkfit stimulus 203
 Check probe fit 71
 Chirp stimulus 140
 Choice bars 46
 Circles 85, 126
 Cleaning 183, 186
 Clear response 91
 Clinical modes 67
 Clinical settings 125
 Clock 213
 Compliance levels 220
 Conditioning the Otoport battery 195
 Connecting the electrodes 39
 Connecting the probe 38, 48
 Contraindications 12
 Control buttons 44
 Controls 147
 Coupler tubes 183
 Critical battery 191

D

- Data entry keypad 26
- Data summary 99
- Date and time 145
- Declared Conformity 216
- Deleting characters 47
- Detailed results 123
- Deviations from the standard 220
- Device Classification 216
- Disconnecting the probe 49
- Dismantling the probe 184
- Display 26, 126
- Downloading 156, 159
- DP High 135
- DP Low 67
- DP Noise rejection calculation 203
- DPOAE test results 81
- DP stimulus calibration 73
- DP test screen 74
- Dual probe result 173

E

- Ear canal size 70
- Ear cup Checkfit 97
- Ear cups 20, 24, 59, 97, 140, 142
- Edit User 155
- Electrical interference 64
- Electrode cable loom 19
- Electrodes 38, 60
- Electrode sockets 30
- Electrode test 175
- Electromagnetic compatibility 218
- Electromagnetic (EM) immunity 218
- End data 151
- End of life management 226
- End print 151
- Entering dates 45, 46
- Environment checks 57
- Error 2 199
- Essential performance 218

F

- Fault message 198
- FFT frequency bin 203
- Fit size indicator 70
- Foreign character table 45
- Fsp 99

G

- Good stimulus 26

H

- Hard reset 47
- Hardware fault messages 199
- Hardware options 214
- Hardware processing and storage 214
- High EEG noise 104
- High impedance 104
- High mains noise 104

I

- Impedance check 93
- Impedance check indicator LEDs 30
- Impedance monitoring 101
- Infant distraction screens 77, 86, 87
- Initial charge 188
- Instrument fault message 198
- Interfaces 213

K

- Keypad 44, 213

L

Language 152
 Last 111
 Latex 226
 Link-Test 67
 Lock-up 197
 Logo 52
 Low battery 191

M

Maximum NLo Sweeps 89
 Memory status 146
 Menu selection buttons 26
 Minimum recordable signal level 79
 Mode 131
 Mode select 53, 125
 Myogenic activity 64

N

NLo sweeps 89
 No Clear Response 81, 91
 Noise level indicator 71
 Noise mode 128
 Noise OK LED 47
 Noise rejection calculation 203
 Noisy 71, 172
 NReject 127

O

Occlusion test 177
 On connect 152
 On/Off power button 26
 Otoport lock-up 197

P

Paper 166
 Pass 171
 Password 54
 Patient details 109
 Patient list 119
 Pausing and cancelling the test 90
 Phthalates 226
 Poor probe fit 81, 91
 Power 214
 Print 151
 Printer battery 168
 Printer fault detection 164
 Printer light summary 165
 Probe 48
 Probe and service accessories 179
 Probe cable clip 179
 Probe fit 58
 Probe socket 26
 Probes safety 185
 Probe test 124, 169
 Probe tips 181

Q

Quality tests 124, 169
 Query 172
 Quick save 107, 150
 Quickstart 40

R

Radio receivers 221
Radio transmitters 221
Real ear test 178
Record 118
Regional standards 222
Regulatory marks 29, 33
Removing the Otoport from the ABR
Module 37
Response frequency bands 205
Response window 205
Result 113
Results 121, 123
Review 110
RF Exposure 221
RFID 221
Ringing 71

S

Safety 13
Sample buffer 203
Sample rate 203
Screen modes 67
Screen settings 125
Selecting levels 130, 134
Service 201
Setup 150
Signal and noise calculation 205
Skin preparation 60
Smart 136
Specific Absorption Rate SAR 221
Standby 189
Start mode 133, 138
Stimulus 203, 204
Stimulus adjustment 71, 73, 74
Stimulus and Noise OK indicators 71
Stimulus LED 47
Stimulus pattern 204
Stimulus repetition rate 205
Stop 133
Suitable environments 218

Summary results 121
Switch on 51
Symbol explanations 227
Symbols 27
System 146
System details 197
System info 153

T

TC 99
Template correlation 99
TEOAE probe tips 181
TEOAE settings 131
TEOAE test results 91
TE Quick 131
TE stimulus adjustment 82
Test mode defaults 143
Test result 81, 91, 103
Test settings 125
Test stop reasons 80
test summary screen 122
Tips 181
Too few bands 81, 91
Training 200

U

Up/down/left/right navigation buttons
26
Use of tips 182
User list 155
Users 153
Utilities 118, 124

V

Volume 147

W

Waveform display 100
Worklist 67, 152